



Administrator's Guide

Monitoring PSIM 2.0 (english)

Last update 09/30/2025

Table of Contents

1	Introduction	7
1.1	Document purpose	7
1.2	Purpose of Monitoring PSIM	7
2	Monitoring PSIM general description.....	8
2.1	Features of Monitoring PSIM	8
2.2	Monitoring PSIM restrictions	8
2.3	General information about Monitoring PSIM as a service.....	8
3	Hardware and software requirements.....	9
3.1	Operating system requirements	9
3.2	Hardware requirements	9
4	Installing, restoring, removing of Monitoring PSIM software package	10
4.1	General description of Monitoring PSIM distribution kit	10
4.2	Installation options.....	10
4.3	Installing Agent of control software.....	12
4.4	Installing Server of control software.....	16
4.5	Installing Additional workplace software	22
4.6	Installing Central server of control software	28
4.7	Installing Additional workplace of CSC software	34
4.8	Repairing Monitoring PSIM	40
4.9	Removing Monitoring PSIM	42
5	Configuring Agent of Control.....	45
5.1	Creating necessary Agent Of Control objects	45
5.2	Configuring the logging subsystem	46
5.3	Configuring the Partition Of Control object.....	47
5.3.1	Configuring the Partition Of Control unique ID	47
5.3.2	Configuring a port for incoming UPS messages	48
5.3.3	Configuring communication between Agent Of Control and Server Of Control	49
5.3.4	Configuring captions.....	52
5.3.5	Configuring the camera list	54

5.3.6	Configuring sensors	57
5.3.7	Configuring alarm groups.....	61
	Configuration for associating events with certain alarm groups	61
	Setting up the configurations for transferred video data	67
	Changing the description of short alarms and long alarm Object disarmed.....	69
	Configuring alarms for monitoring the object state on the Agent of Control side	71
5.4	Connecting to uninterrupted power supplies	74
5.4.1	Configuring StateUPS	74
5.4.2	Installing the software from the UPS vendor	74
5.4.3	Configuring the PowerChute plus utility	82
5.4.4	Example of configuration of event distribution	85
5.5	Working with Agent of control without Windows administration rights	87
6	Configuring Server of Control.....	89
6.1	Creating necessary Server Of Control objects	89
6.2	Configuring a connection	90
6.3	Configuring logging subsystem.....	91
6.3.1	Specifying storage time for event log	93
6.3.2	The Event Viewer utility	93
6.4	Configuring reaction to snapshots and videos.....	95
6.5	List of Additional workplaces	97
6.6	Sending confirmations of alarm acceptance.....	101
6.7	Working with Server of Control without Windows administration rights	102
6.8	Configuring sound notification at Server of Control	103
6.8.1	Configuring sound notification at Servers Of Control in a general way	103
6.8.2	Configuring sound notification at Server Of Control for various alarm groups.....	104
6.9	Configuring the Server of Control from another server in a distributed configuration	106
6.10	Sending alarm events via Telegram bot	109
7	Configuring Central Server of Control.....	114
7.1	General principles of the Central Server of Control software	114
7.2	Configuring the FTP server for the Central Server of Control operation.....	116
7.3	Creating the Central Server Of Control object.....	120
7.4	Configuring the Servers of Control tracking	121

7.4.1	Adding the Server Of Control.....	121
7.4.2	Editing the Server Of Control.....	123
7.4.3	Deleting the Server Of Control	124
7.5	Configuring the Additional workplace of CSC connection rights to the Central Server of Control	125
7.5.1	Adding the Additional workplace of CSC	125
7.5.2	Editing the Additional workplace of CSC	127
7.5.3	Deleting the Additional workplace of CSC	128
7.6	Advanced settings of the Central Server of Control	129
7.7	Working with Central Server Of Control without Windows administration rights	130
7.8	Configuring the Central Server Of Control from another server in a distributed configuration.....	130
8	Configuring Additional workplace and Additional workplace of CSC.....	135
8.1	List of Servers of Control/CSC	135
8.1.1	Interface of Additional workplace configuration tool.....	135
8.1.2	Adding Server of Control to the list.....	138
8.1.3	Selecting active Server of Control	142
8.2	Working with Additional workplace/Additional workplace of CSC without Windows administration rights	142
8.3	Creating and configuring Data Gateway.....	142
9	Configuring the Monitoring PSIM fault tolerance.....	144
10	Configuring the special mode of Monitoring operation with ACFA PSIM.....	145
10.1	General information about special mode of Monitoring PSIM operation with ACFA PSIM	145
10.2	Configuring the special mode of Monitoring PSIM operation with ACFA PSIM on the Server of Control side	145
10.3	Configuring the special mode of Monitoring PSIM operation with ACFA PSIM on the Agent of Control side	147
10.4	Operating procedure	149
11	Data loader for Monitoring	150
11.1	Server of Control communication module	150
11.2	Data loader	150
11.3	Connecting to the database	152

11.4	Removing errors.....	152
11.5	Removing events from the database	152
11.6	Setting the log storage period	153
11.7	Configuring automated video clip loading.....	154
11.8	Specifying the export directory	154
12	Configuration of the Monitoring PSIM interface.....	156
12.1	General information about the Monitoring PSIM interface	156
12.2	Configuring the Monitoring interface object	156
12.3	Configuring the Search in archive object.....	162
12.4	Configuration of the Monitoring reports object	162
13	Configuring audio calls from the Monitoring interface	164
13.1	General information.....	164
13.2	Configuring audio calls from the Monitoring interface.....	164
14	Configuring special operation mode joint with Auto PSIM.....	167
14.1	Configuration on the Agent Of Control side	167
14.2	Configuration on the Server Of Control side	168
15	Appendix 1. Interfaces	170
15.1	Settings panel of the Agent Of Control object.....	170
15.2	Settings panel of the Partition Of Control object.....	171
15.3	Settings panel of the Server Of Control object.....	175
15.4	Settings panel of the Monitoring interface object.....	180
15.5	Settings panel of the Monitoring reports interface object.....	192
15.6	Settings panel of the Search in archive interface object	196
15.7	Settings panel of the Central Server Of Control object.....	201
16	Appendix 2. Sample scripts	204
16.1	Sample script for processing Server of Control command on Agent of Control.....	204
16.2	Sample script for setting custom filter in the Log panel.....	205
16.3	Sample script for stopping camera recording.....	206
16.4	Sample scripts for processing alarm confirmations	208
16.5	Sample script to export filtered data from the Log panel to .xls.....	209

16.6	Sample script to show and hide Search license plates window	209
16.7	Sample scripts for the special mode of Monitoring PSIM operation with ACFA PSIM	210
16.7.1	Sample script for configuring the interaction between the Monitoring PSIM and the Apollo integration module.....	210
16.7.2	Sample scripts for determining the current state of the zones of the Apollo object on the Agent of Control side.....	211
16.8	Sample scripts for determining the current state of the relay on the Agent of Control side.....	214
16.9	Sample script for creating a hardware failures report.....	215
16.10	Sample script for creating an alarms report.....	216

1 Introduction

On the page:

- [Document purpose](#)
- [Purpose of Monitoring PSIM](#)

1.1 Document purpose

This document, *Monitoring PSIM. Administrator's Guide*, is a reference aid for system administrators, configuration and installation specialists, and users with administrator rights on the *Monitoring PSIM* of technical condition software (hereinafter referred to as *Monitoring PSIM*).

This guide describes the following:

1. Purpose of *Monitoring PSIM*.
2. Hardware and software requirements for *Monitoring PSIM*.
3. Installation procedure for *Monitoring PSIM*.
4. Configuration of *Monitoring PSIM* components.

1.2 Purpose of Monitoring PSIM

Monitoring PSIM is designed to automate the activities of personnel at service companies involved in the operation of *Axxon PSIM*-powered video surveillance systems. The purpose of *Monitoring PSIM* is to improve the quality of operation for such video surveillance systems.

2 Monitoring PSIM general description

2.1 Features of Monitoring PSIM

Monitoring PSIM receives, records, and visualizes messages about the state of security system components, based on the following key parameters:

1. Camera operability.
2. Network functioning.
3. Operability of video subsystem software.
4. Amount of recorded video.
5. Hard disk operability.
6. Operability of fire/security and access control systems.
7. UPS signals.

In addition, *Monitoring PSIM* allows you to control the actions of *Monitoring PSIM* operators: recording is performed of whether an alarm has been accepted, how much time passed before the alarm was accepted, etc. The built-in system of statistical and analytical reports allows you to generate reports on the system operation: reports on alarms, downtime, statistics on security system operation, and more.

Note

If there is no activation key, then *Monitoring PSIM* operates in the demo mode for two months from 8:00 am to 12:00 am.

2.2 Monitoring PSIM restrictions

In the *Monitoring PSIM* software package restrictions are imposed when creating systems of technical condition *Monitoring PSIM*:

1. Maximal number of **Agent Of Control** objects that can be connected to a *Server of Control* is 2000.
2. Maximal number of **Partition Of Control** objects being child objects for an **Agent of Control** is 255.
3. Maximal number of cameras which a **Partition Of Control** can handle is 64.
4. Maximal number of cameras which a **Agent Of Control** can handle is 320.

2.3 General information about Monitoring PSIM as a service

Monitoring PSIM software, installed as a service (see [Installing, restoring, removing of Monitoring PSIM software package](#)), is launched before user authorization in Windows OS and before launching Windows applications (including the Explorer, which is used to launch interfaces of both Windows OS and various applications installed on server).

When the active account is changed, the following *Monitoring PSIM* modules are restarted:

- On *Agent of Control* — videosrv.exe;
- On *Server of Control* — videosrv.exe and loadersstv.exe;
- On *Central Server of Control* — CentralNetServer.exe.

If *Monitoring PSIM* is installed as a service, and the connection to the database is established using Windows credentials, then to ensure the operation on any user account other than the one who installed *Monitoring PSIM*, the user should have the appropriate rights to SQL Server.

3 Hardware and software requirements

On the page:

- [Operating system requirements](#)
- [Hardware requirements](#)

3.1 Operating system requirements

Monitoring PSIM is provided as executable modules that can be run on the operation systems supported by the *Axxon PSIM* software (see the [Operating system requirements](#) chapter in the *Axxon PSIM* software Administrator's Guide).

The software is compatible with standard operating system settings. On Windows Vista and later, UAC must be disabled. In Windows 8, 8.1 and 10 it is necessary to configure security policies in order to entirely disable UAC (configuring security policies is described in the [Axxon PSIM software Administrator's Guide](#)).

For the *Server of Control* and the *Central Server of Control* to operate, there must be an available database server. During installation of *Axxon PSIM*, MS SQL Server 2014 Express is installed to a "clean" (fresh) system.

The *Server of Control* and the *Central Server of Control* are compatible with the following servers:

- MS SQL Server 2008 R2,
- MS SQL Server 2012,
- MS SQL Server 2014.

3.2 Hardware requirements

Monitoring PSIM can run on PCs that meet the following minimum hardware requirements:

- Intel Core i5 750 CPU,
- 2 GB RAM,
- 200 GB HDD,
- NIC,
- Graphics card with overlay support.

4 Installing, restoring, removing of Monitoring PSIM software package

4.1 General description of Monitoring PSIM distribution kit

Monitoring PSIM is supplied as a software installation package (distribution kit). The current version of the distribution kit can be downloaded from the official [AxxonSoft](#) website.

The distribution kit contains all the necessary software components for installing the *Monitoring PSIM* software package on a base computer.

The distribution kit allows you to install, restore and remove the *Monitoring PSIM* software package.

Attention!

- Prior to installing, restoring or removing the *Monitoring PSIM* software package, the *Axxon PSIM* operation should be shut down.
- Administrator rights are required for installing, restoring or removing *Monitoring PSIM*.

4.2 Installation options

Monitoring PSIM can be installed in one of the following configurations:

Installation type	Purpose	License features	Additional components	Base Axxon PSIM installation type
Agent of control	Is to be installed on the object for which receiving, recording, and visualizing messages about the state of security system components is required.	The program key, psim.sec, should contain the Agent Of Control object.	In addition to <i>Agent of Control</i> modules, the VideoSrv communication program is installed. It interacts with similar programs on the <i>Server of Control</i> .	Server/RAW

Server of control	Is to be installed on the object from which the <i>Agents of Control</i> are monitored.	The program key, psim.sec, should contain the Server Of Control object.	<p>In addition to <i>Agent of Control</i> modules the following components are installed:</p> <ol style="list-style-type: none"> 1. VideoSrv communication module. It interacts with similar programs on the <i>Agent of Control</i>. 2. Data loader for <i>Monitoring PSIM</i> to record information collected by VideoSrv into the database.
Additional workplace	This is the <i>Server of Control</i> version which is installed without additional components and connects to the existing database of the main <i>Server of Control</i> while interface objects are created on the local computer.	<p><i>Axxon PSIM</i> distributed system configuration is not required for the additional workplace operation.</p> <p>The Additional workplace object is to be specified in the psim.sec license key that is located on <i>Server of Control</i> in order to allow using the <i>Additional workplace</i> software.</p>	-


Central server of control	Allows to combine several <i>Servers of Control</i> into a single system.	The program key, psim.sec, should contain the Central Server Of Control object.	In addition to <i>Central Server of Control</i> modules the following components are installed: <ol style="list-style-type: none"> 1. CentralNetServer communication module. It interacts with VideoSrv modules on the <i>Server of Control</i>. 2. Data loader for <i>Central Server of Control</i> which records the information received from CentralNetServer into the database.
Additional workplace of CSC	This is the <i>Central Server of Control</i> version which is installed without additional components and connects to the existing database of the main <i>Central Server of Control</i> while interface objects are created on the local computer.	<p><i>Axxon PSIM</i> distributed system configuration is not required for the additional workplace operation.</p> <p>The Additional workplace of CSC object is to be specified in the psim.sec license key that is located on <i>Central Server of Control</i> in order to allow using the <i>Additional workplace</i> software.</p>	-

4.3 Installing Agent of control software


The *Monitoring PSIM* is installed as an extension to the *Axxon PSIM* software. Information about the compatibility of the *Axxon PSIM* software versions and *Monitoring PSIM* is presented in the [General information about product releases and versions compatibility](#) section.

To install *Monitoring PSIM* in the *Agent of control* software configuration, do the following:


1. In the root directory of the distribution package, run the setup.exe executable file.
2. To continue the installation process, click the **Next** button.

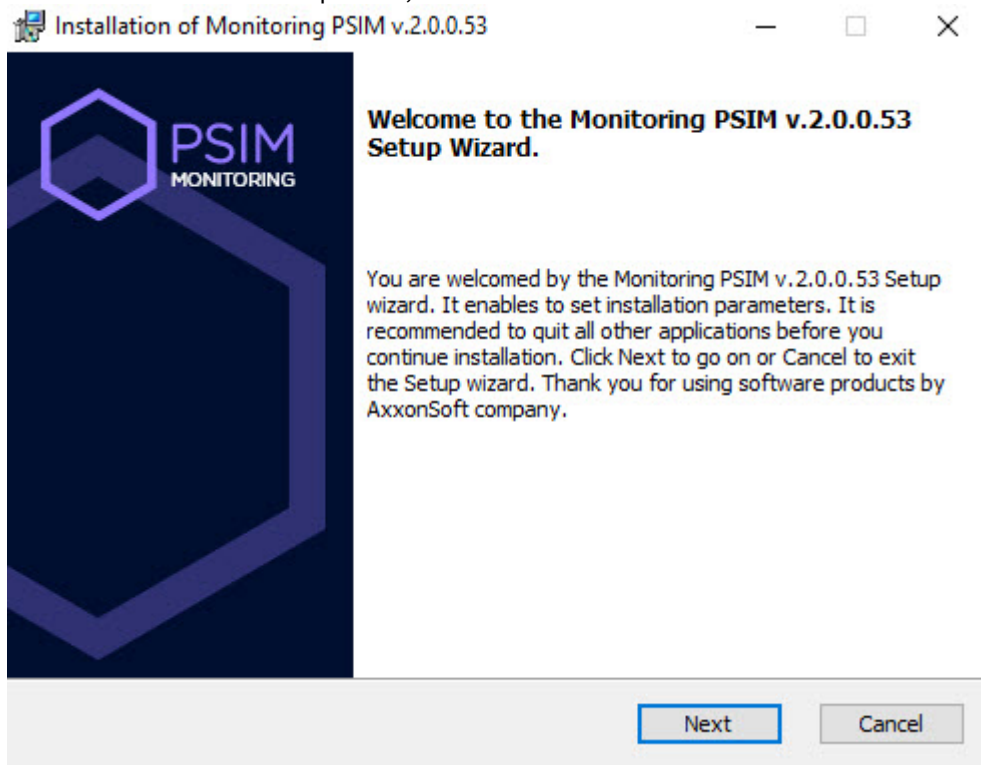


3. Read carefully the terms of the license agreement. Then set the switch to the **I accept the terms of the License agreement** position and click the **Next** button.

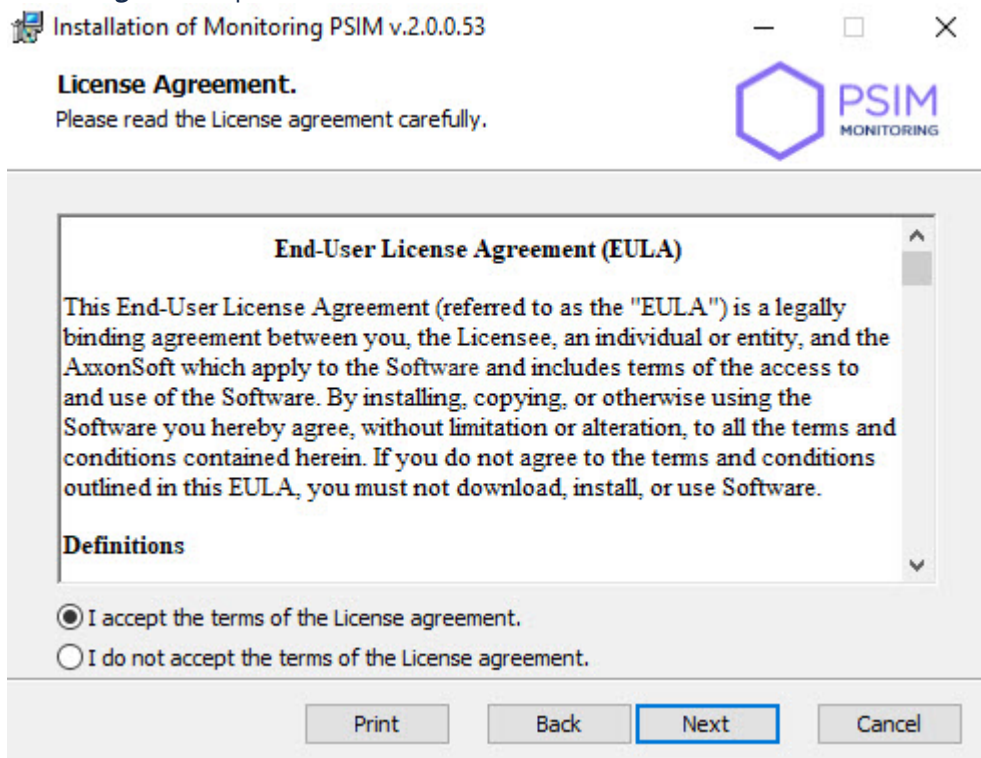


4. Select the **Agent of control** installation type and click the **Next** button.

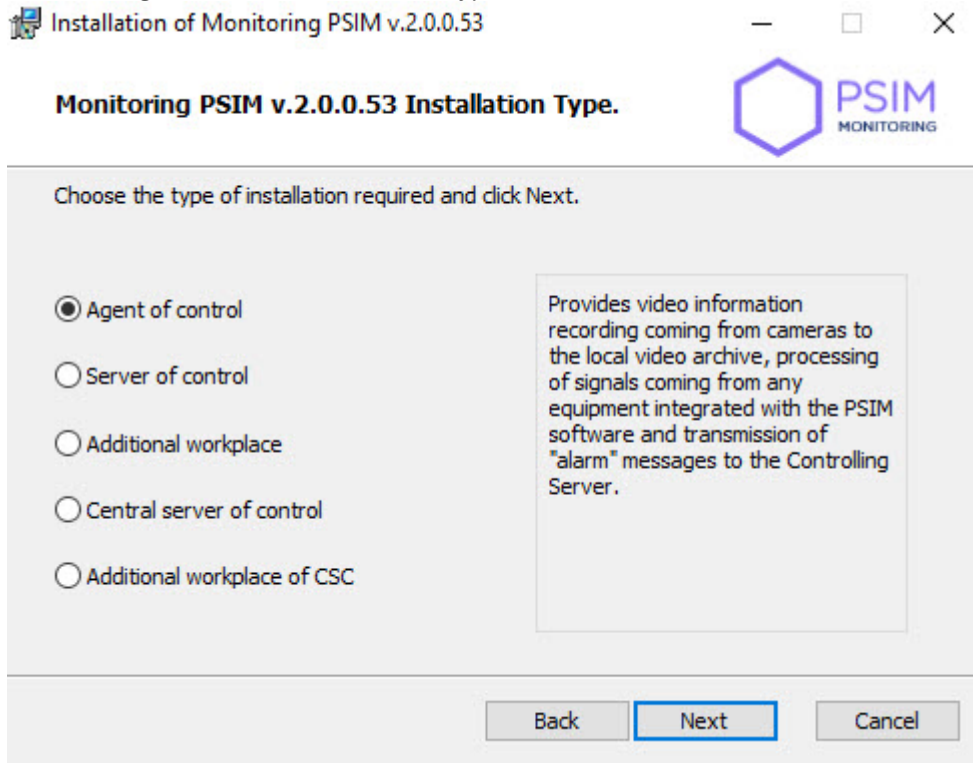


5. If *Axxon PSIM* is installed as a service, and you want to start *Monitoring PSIM* as a service, then set the **Install Monitoring PSIM as a service** checkbox and click the **Next** button (for more details, see [General information about Monitoring PSIM as a service](#)).

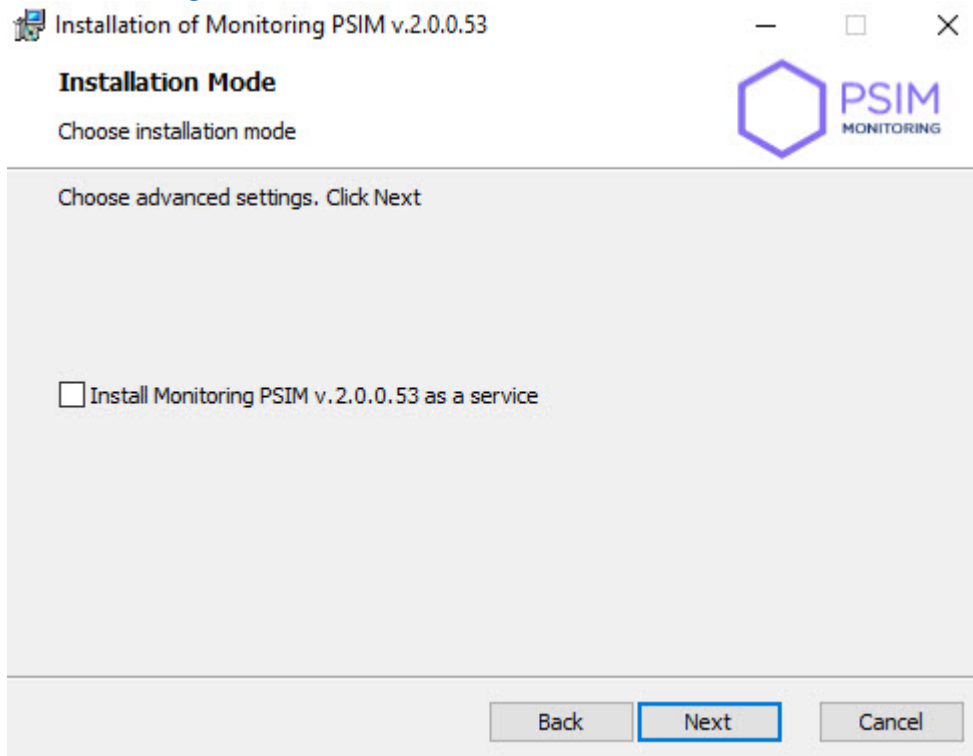


- Click the **Install** button to start the installation process.

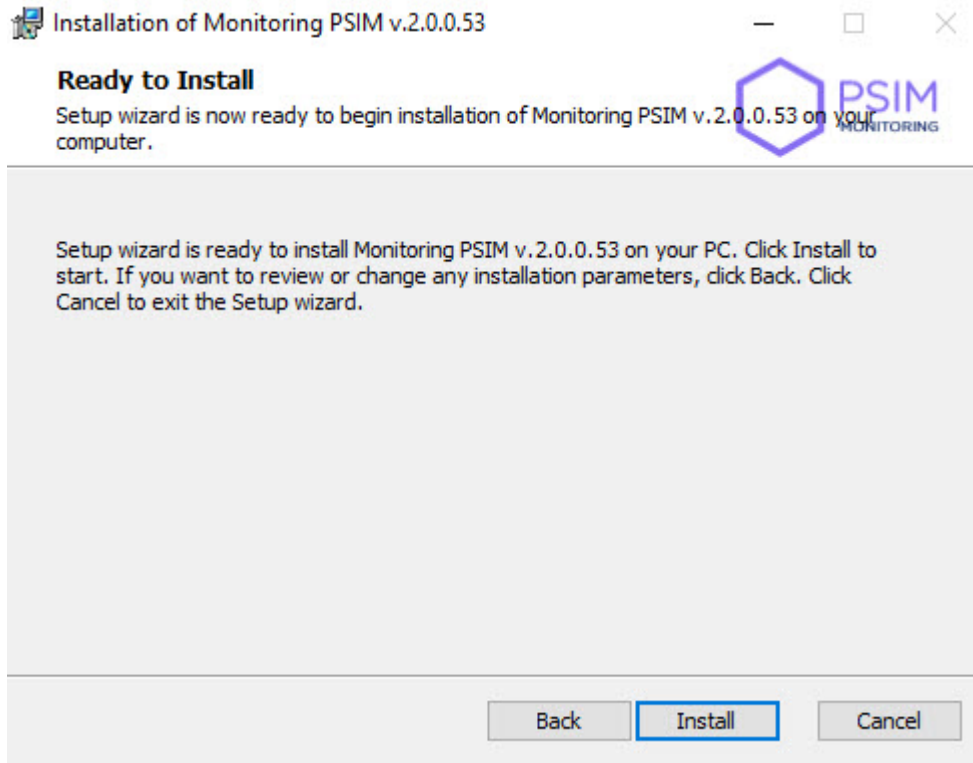

As a result, the system starts copying the required files of *Monitoring PSIM* to the computer's hard disk.

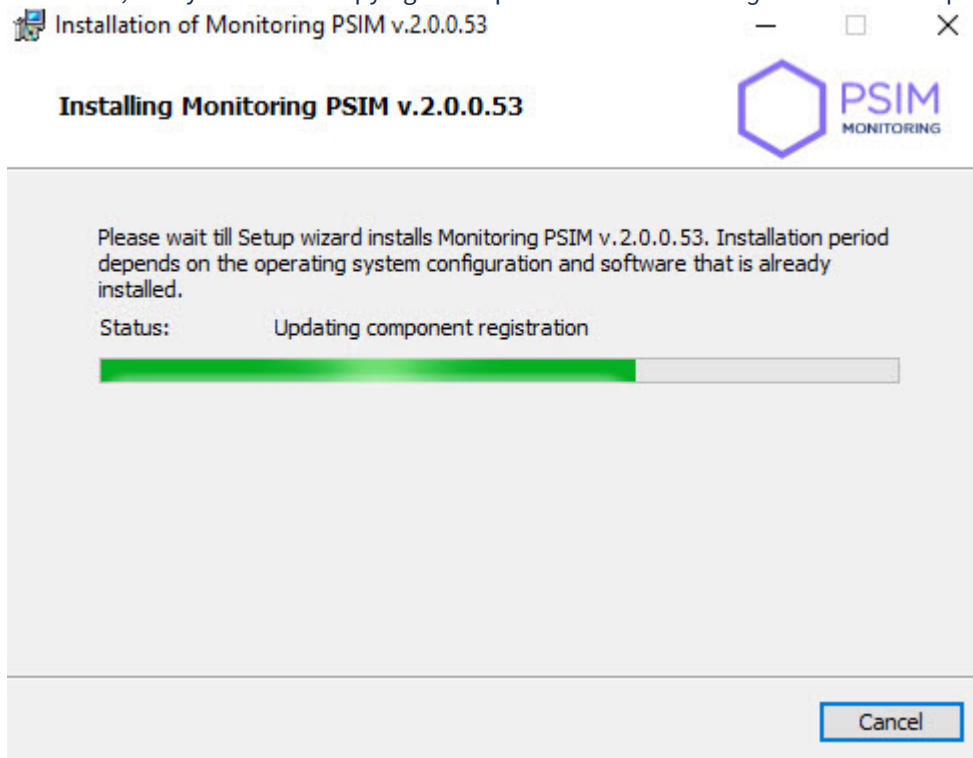

7. After the system successfully copies the *Monitoring PSIM* components, the message about completing the installation process is displayed. Next, click the **Finish** button.

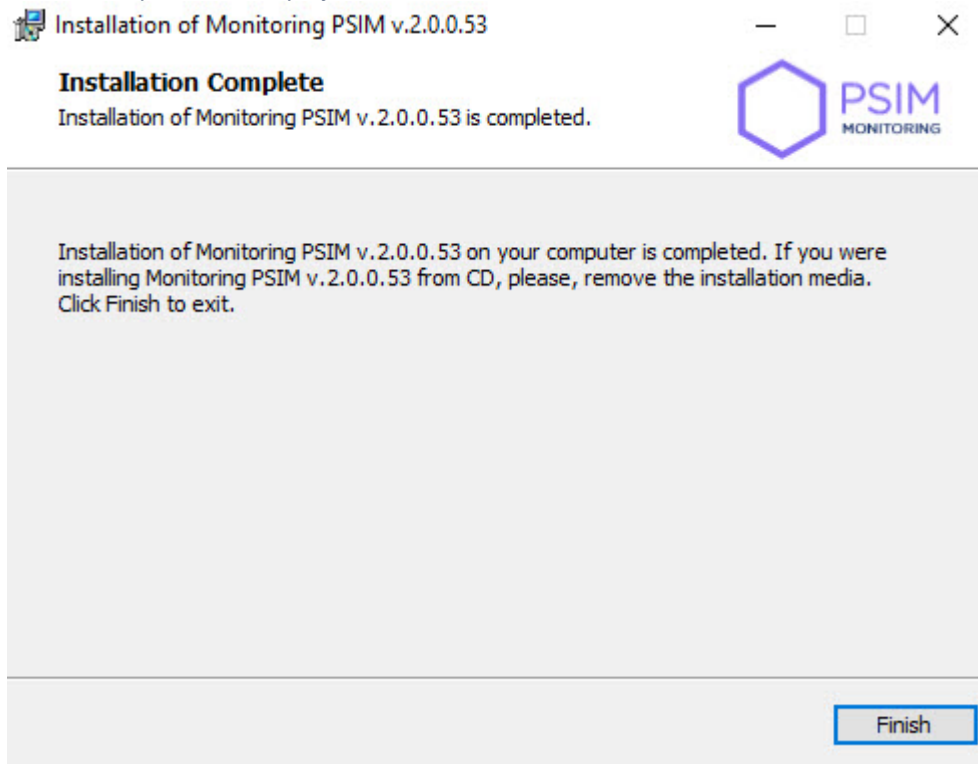

Installing the *Agent of control* software is complete.


4.4 Installing Server of control software

The *Monitoring PSIM* is installed as an extension to the *Axxon PSIM* software. Information about the compatibility of the *Axxon PSIM* software versions and *Monitoring PSIM* is presented in the [General information about product releases and versions compatibility](#) section.


To install *Monitoring PSIM* in the *Server of control* software configuration, do the following:

1. In the root directory of the distribution package, run the setup.exe executable file.


- To continue the installation process, click the **Next** button.

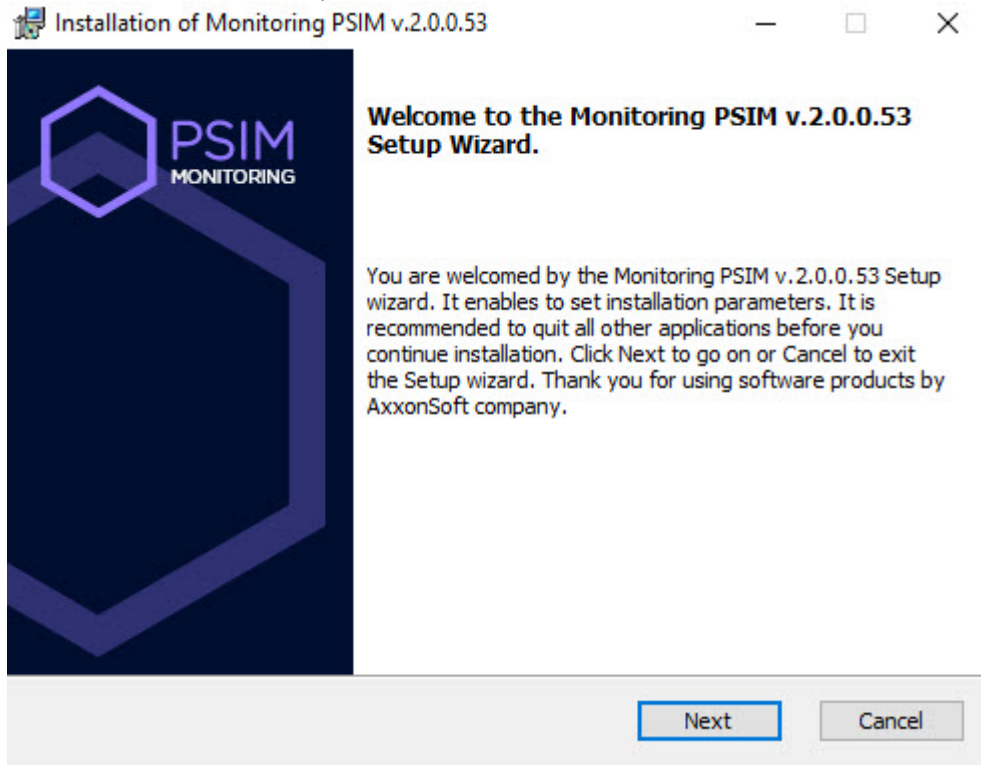


- Read carefully the terms of the license agreement. Then set the switch to the **I accept the terms of the License agreement** position and click the **Next** button.

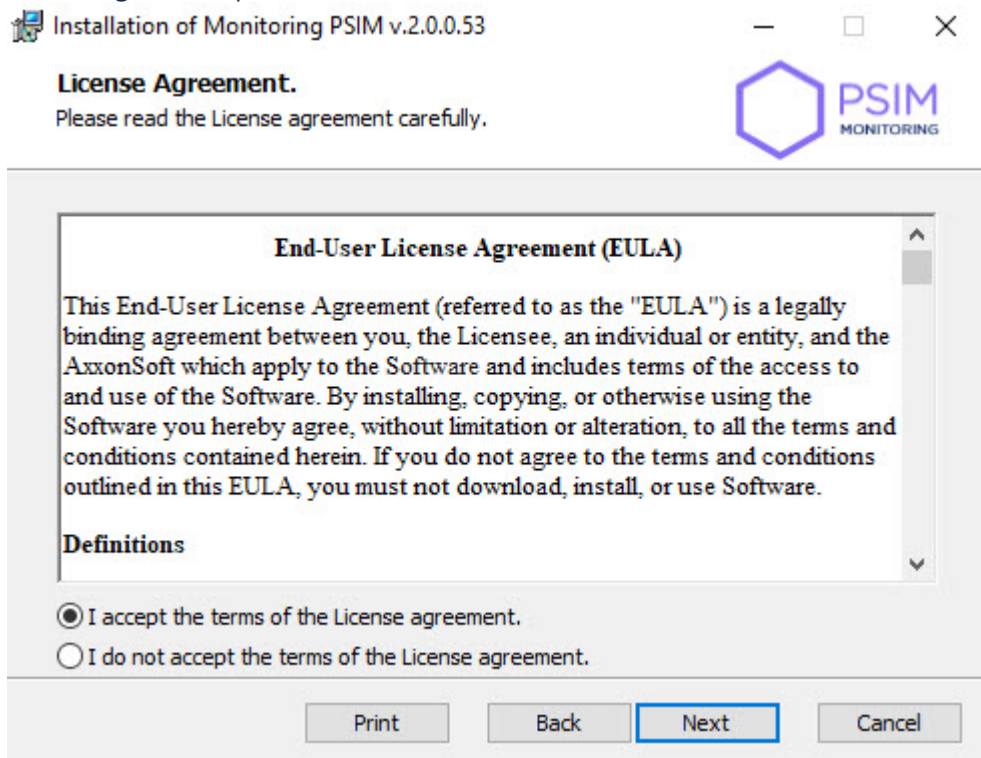

4. Select the **Server of control** installation type and click the **Next** button.

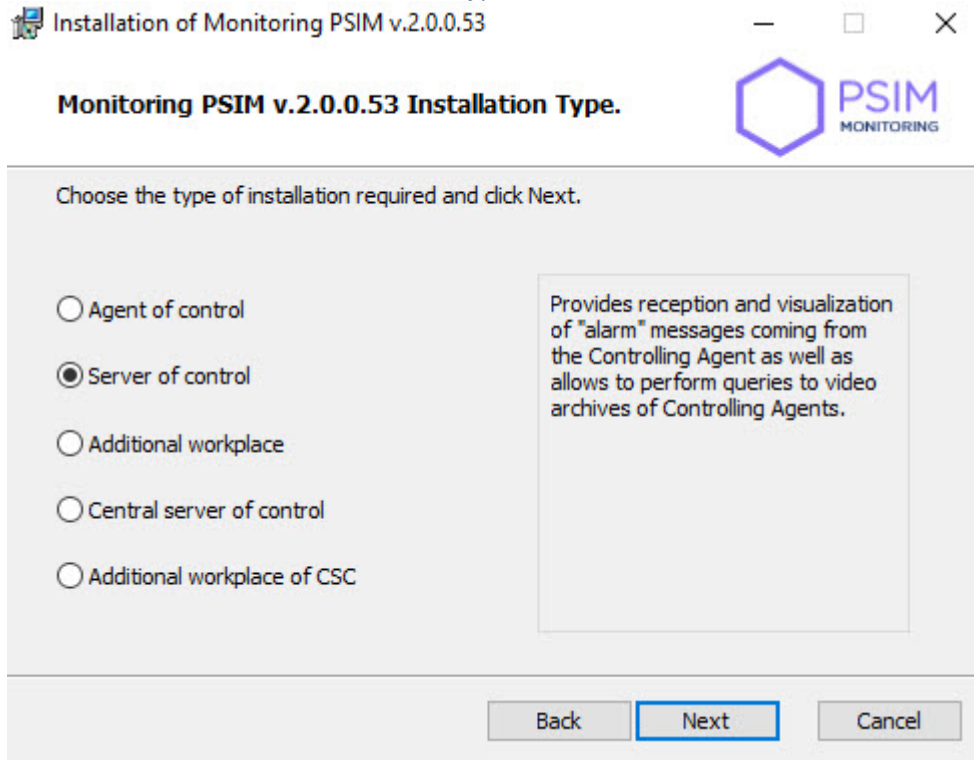

5. If *Axon PSIM* is installed as a service, and you want to start *Monitoring PSIM* as a service, then set the **Install Monitoring PSIM as a service** checkbox and click the **Next** button (for more details, see [General information about Monitoring PSIM PSIM as a Service](#)).

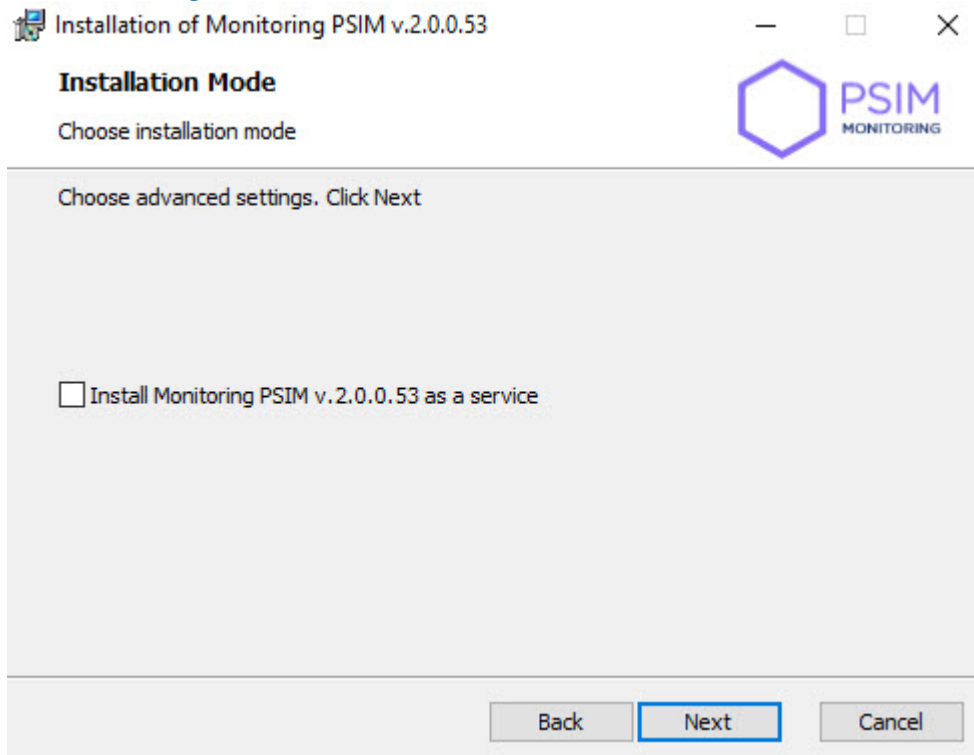

6. Select the MS SQL database server and specify the connection parameters. For more details, see [Installation of Axxon PSIM™ as a Server/Remote Administrator's workplace](#). To continue the installation process, click the **Next** button.

Note

In the **Select database Server from the drop-down list** field, you must specify the **127.0.0.1** value of the IP address without using the computer names and local value. Otherwise, the *Server of control* software loses connection with its local database when the network cable is disconnected.

Installation of Monitoring PSIM v.2.0.0.53

Select Database Server

Select database Server and authentication method.

Select database Server from the drop-down list.

127.0.0.1\SQLEXPRESS2014

Choose user identification procedure based on the present user account or SQL Server identity check.

Windows user account

Use the following user name and password:

User name: sa


Password: [Masked]

Back Next Cancel


7. In the **Database** field, specify the name of the database or select it in the list of existing databases from the right and click the << button. Click the **Next** button.

Note


By default, the name of the database is "MonitorSSTV", and its files are stored in the SQL Server folder.

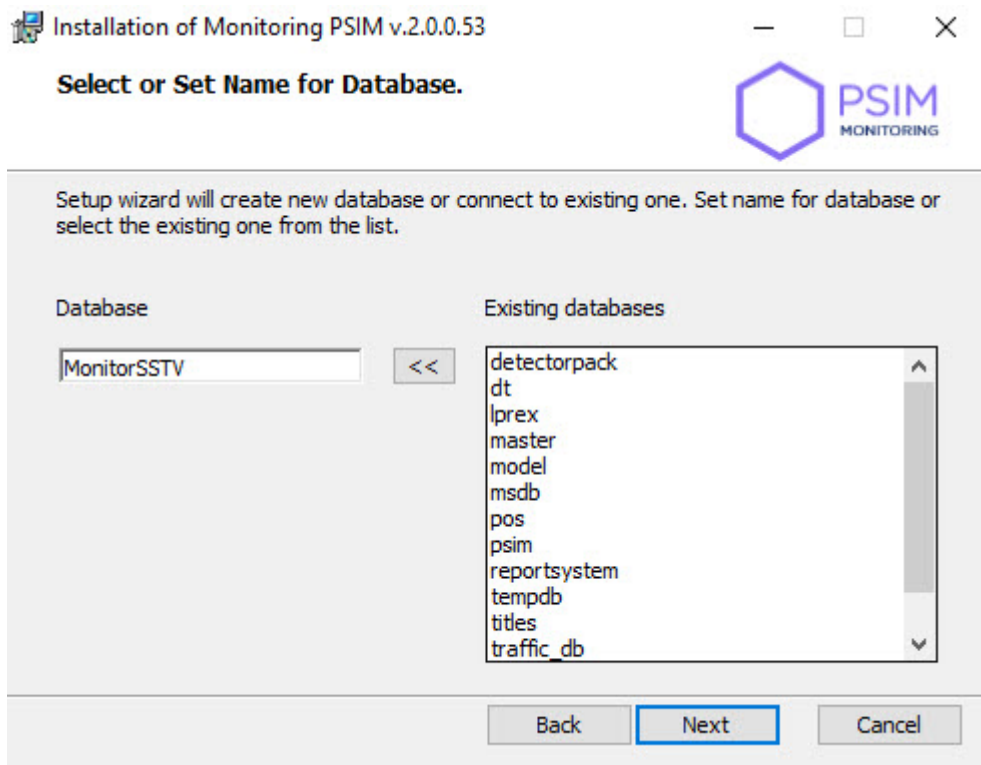


- Click the **Install** button to start the installation process.

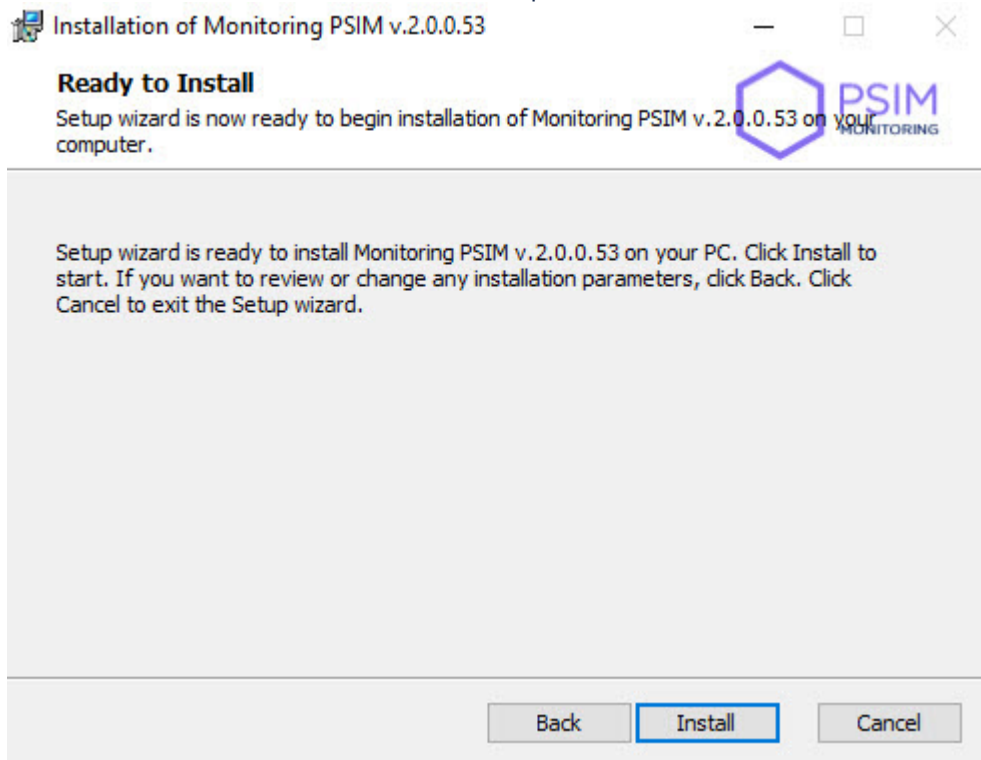

As a result, the system starts copying the required files of *Monitoring PSIM* to the computer's hard disk.

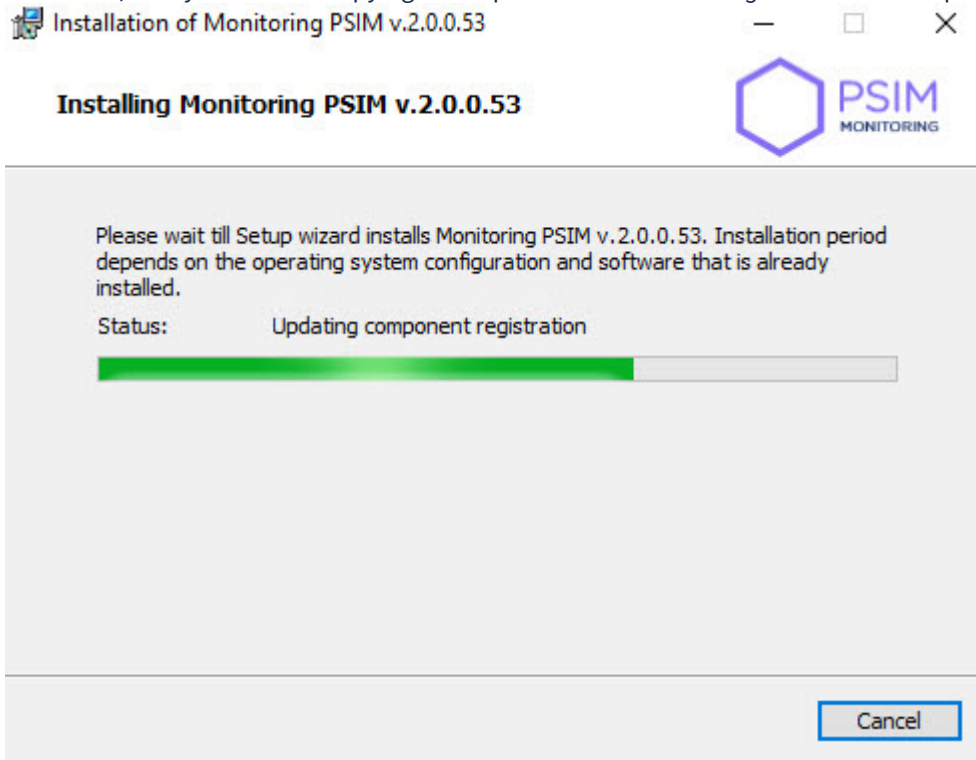

9. After the system successfully copies the *Monitoring PSIM* components, the message about completing the installation process is displayed. Next, click the **Finish** button.

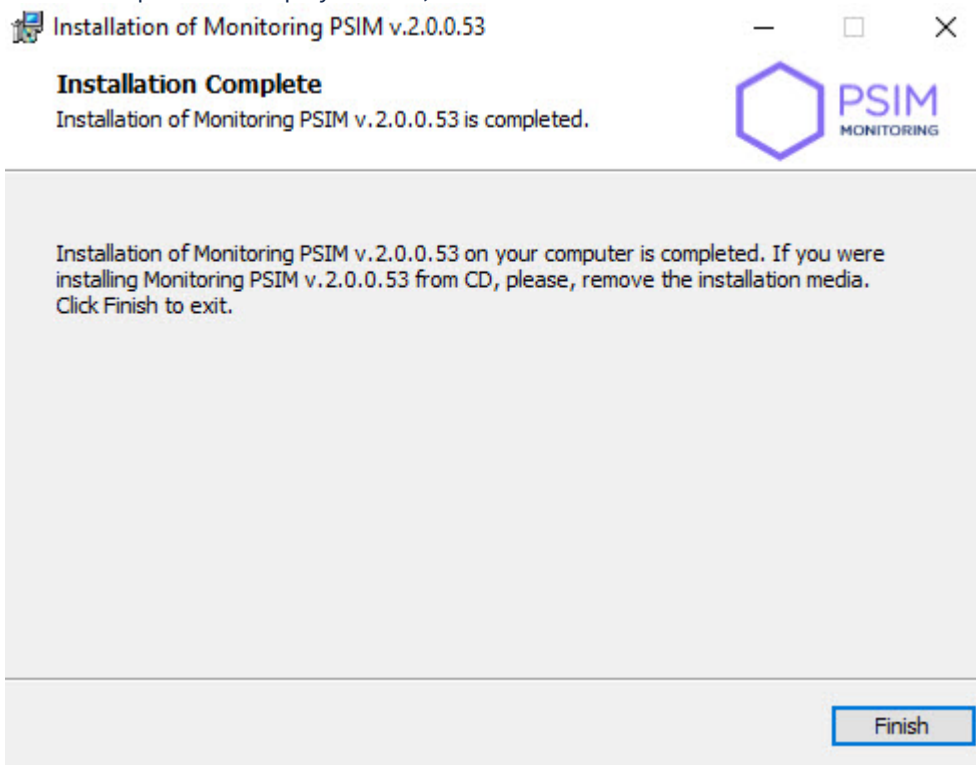


Installing the *Server of control* software is complete.

4.5 Installing Additional workplace software


The *Monitoring PSIM* is installed as an extension to the *Axxon PSIM* software. Information about the compatibility of the *Axxon PSIM* software versions and *Monitoring PSIM* is presented in the [General information about product releases and versions compatibility](#) section.

To install *Monitoring PSIM* in the *Additional workplace* software configuration, do the following:


1. In the root directory of the distribution package, run the setup.exe executable file.
2. To continue the installation process, click the **Next** button.

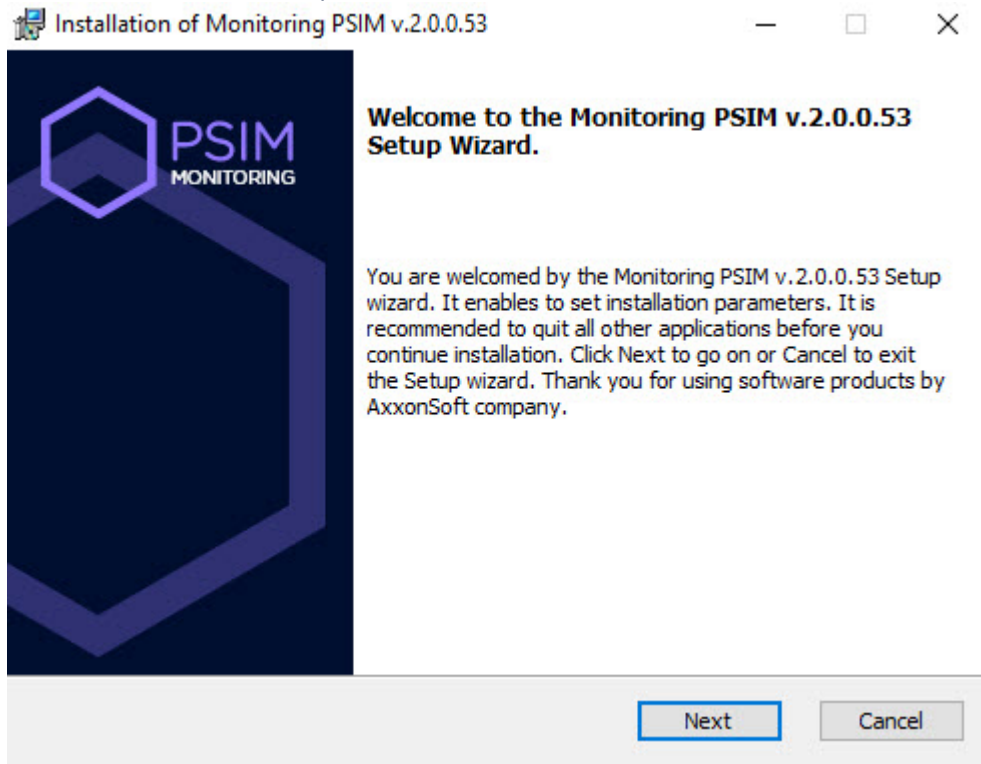

3. Read carefully the terms of the license agreement. Then set the switch to the **I accept the terms of the License agreement** position and click the **Next** button.

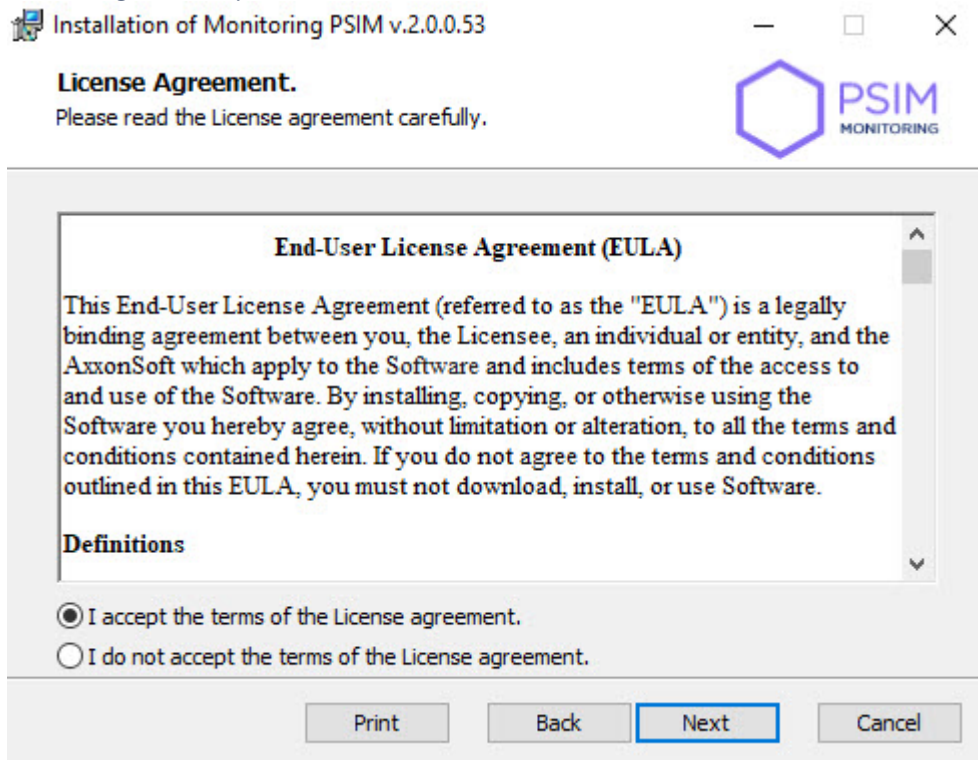

4. Select the **Additional workplace** installation type and click the **Next** button.

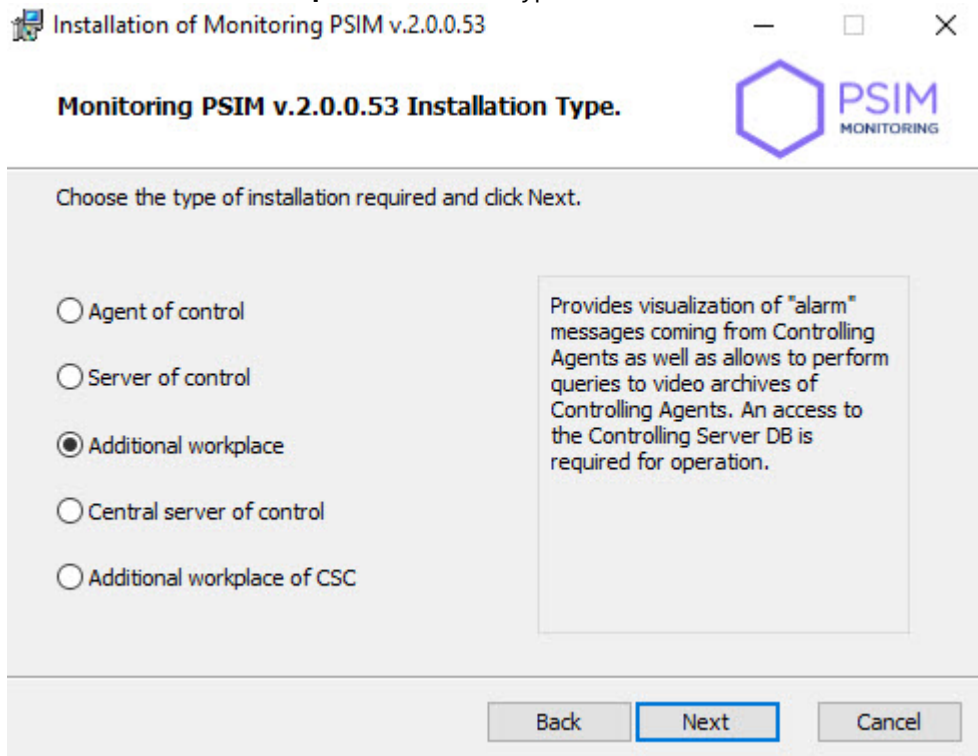

5. Select the MS SQL database server and specify the connection parameters. For more details, see [Installation of Axxon PSIM as a Server/Remote Administrator's workstation](#). To continue the installation process, click

the **Next** button.

Installation of Monitoring PSIM v.2.0.0.53

Select Database Server

Select database Server and authentication method.

Select database Server from the drop-down list.

192.168.56.1\SQLEXPRESS2014

Choose user identification procedure based on the present user account or SQL Server identity check.

Windows user account

Use the following user name and password:

User name: sa


Password: [Masked]

Back Next Cancel


- In the **Database** field, specify the name of the database or select it in the list of existing databases from the right and click the << button. Click the **Next** button.

Note

By default, the name of the database is "MonitorSSTV", and its files are stored in the SQL Server folder.

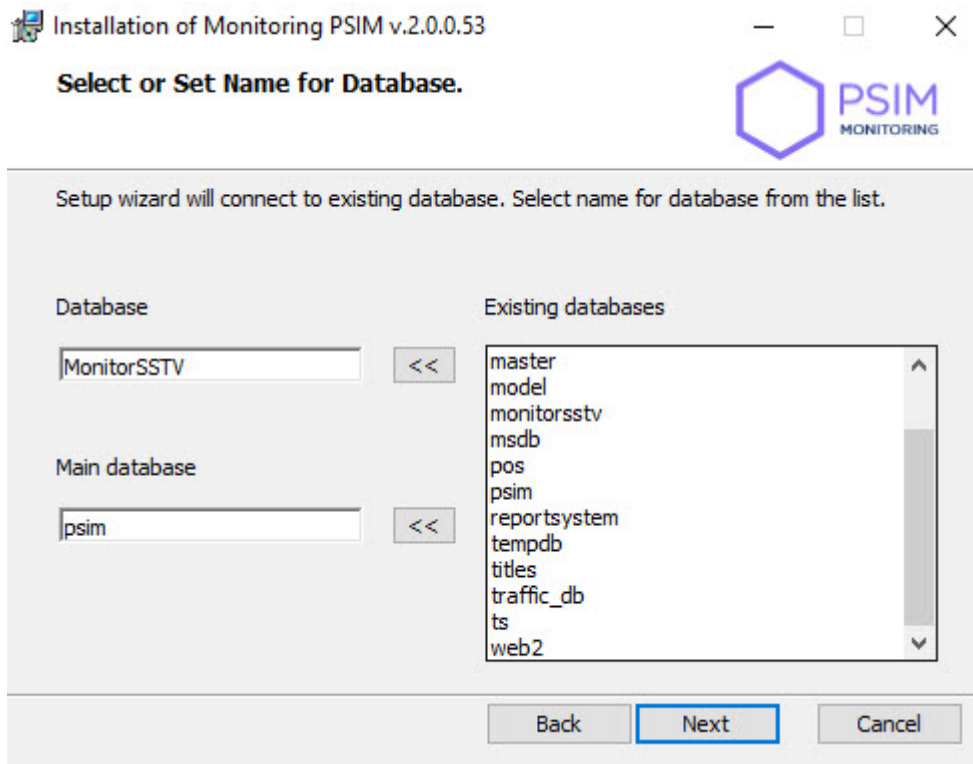

- Specify the export catalog path. This catalog will contain video data received from *Agent of Control*. Click the **Next** button.

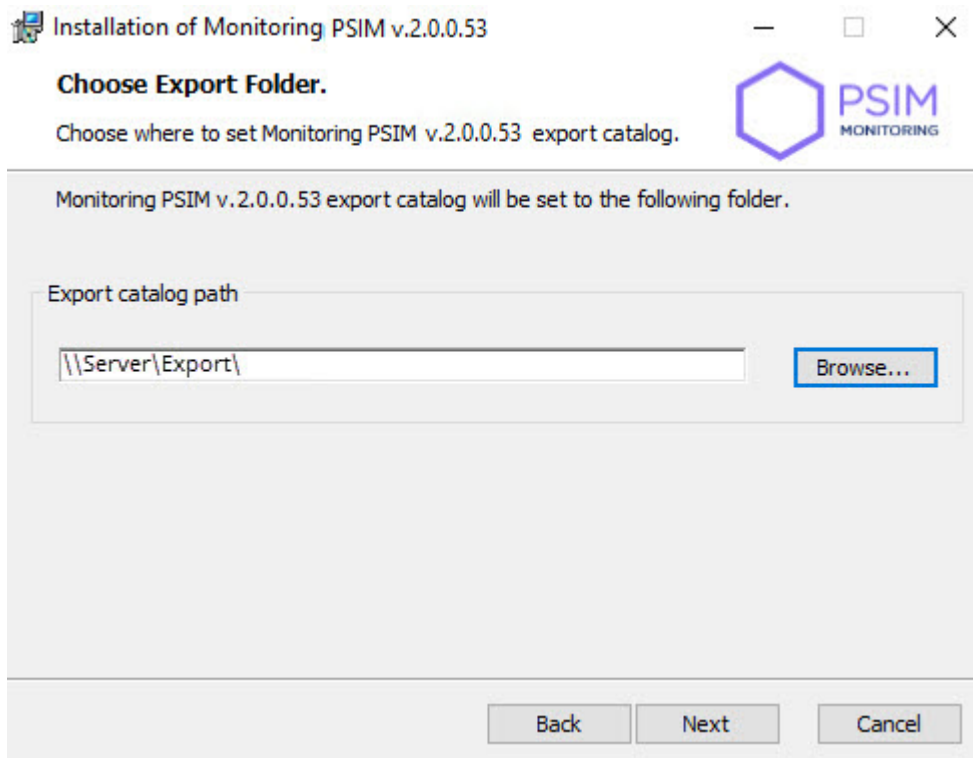

- Specify the IP address and port to connect to the *Server of Control* videosrv communication module. Click the **Next** button.


Note

We highly recommend changing the default values for the **Export catalog path** and **IP address** parameters on steps 7-8. Otherwise, after the installation is completed, you must configure Additional workplace (see [Configuring Additional workplace](#) and [Additional workplace of CSC](#)).

Installation of Monitoring PSIM v.2.0.0.53

Setting up connection to communication module.

Please input ip address and port.



Connection to communication module would be set according to the following values.


Videosrv settings

IP address


Port

Back Next Cancel


- Click the **Install** button to start the installation process.

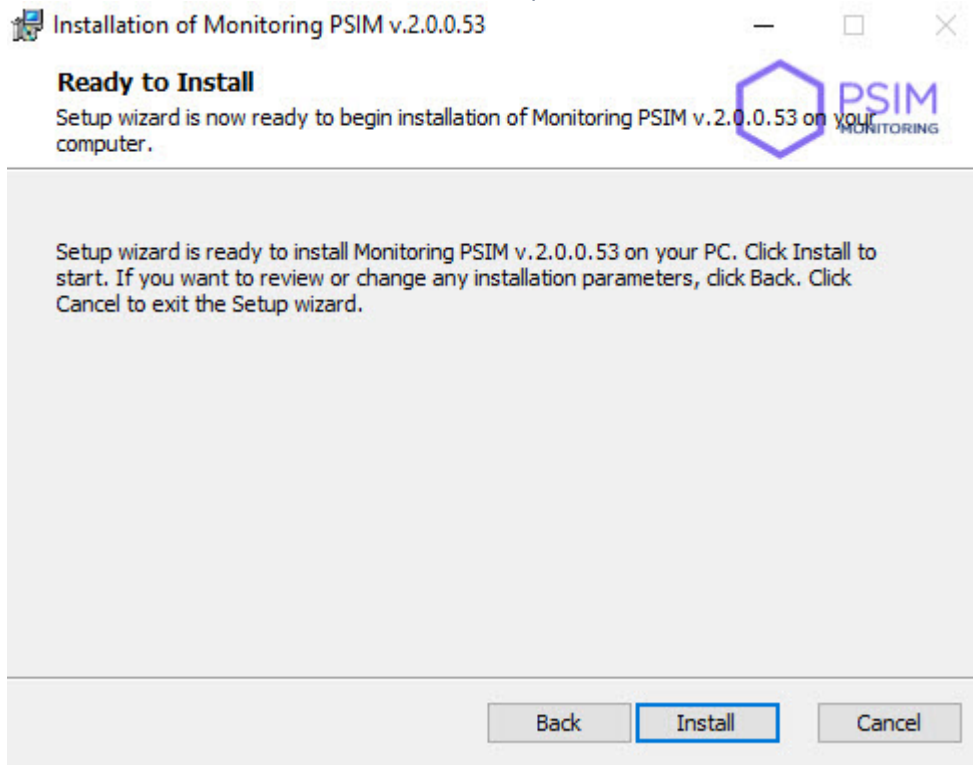

As a result, the system starts copying the required files of *Monitoring PSIM* to the computer's hard disk.

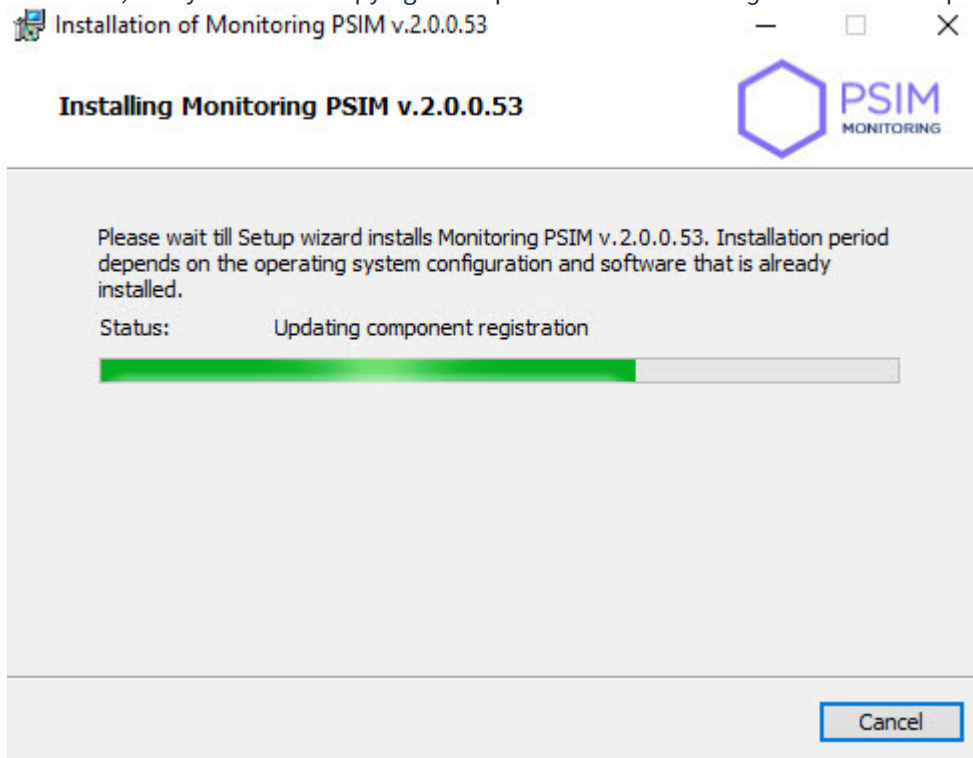

10. After the system successfully copies the *Monitoring PSIM* components, the message about completing the installation process is displayed. Next, click the **Finish** button.

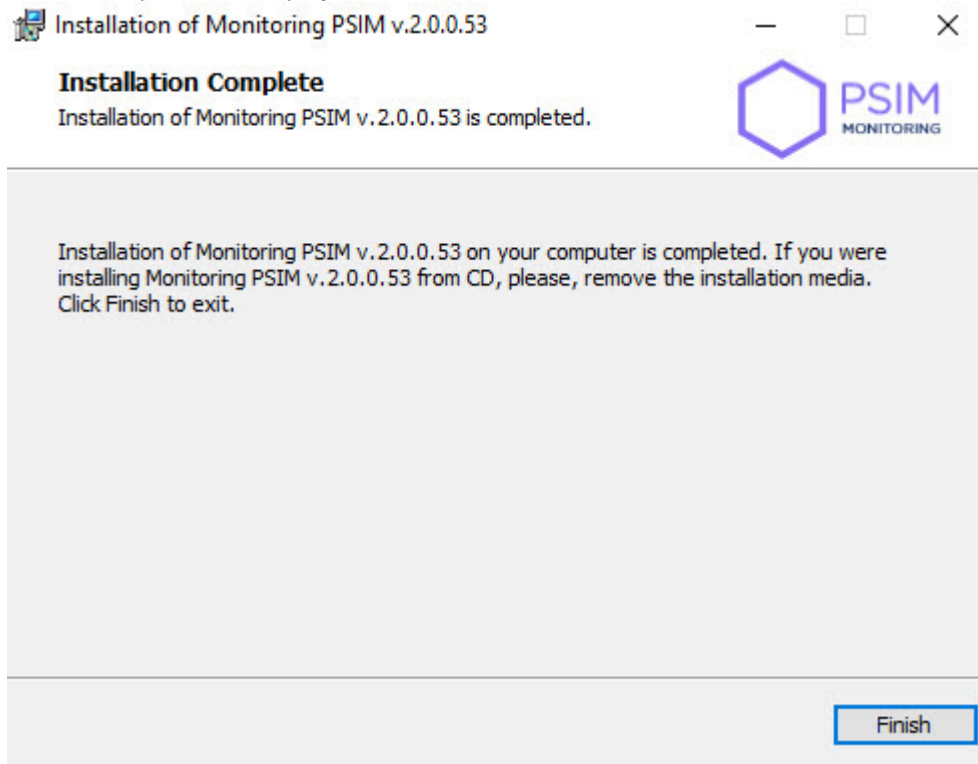

Installing the *Additional workplace* software is complete.


4.6 Installing Central server of control software

The *Monitoring PSIM* is installed as an extension to the *Axxon PSIM* software. Information about the compatibility of the *Axxon PSIM* software versions and *Monitoring PSIM* is presented in the [General information about product releases and versions compatibility](#) section.


To install *Monitoring PSIM* in the *Central server of control* software configuration, do the following:

1. In the root directory of the distribution package, run the setup.exe executable file.


- To continue the installation process, click the **Next** button.

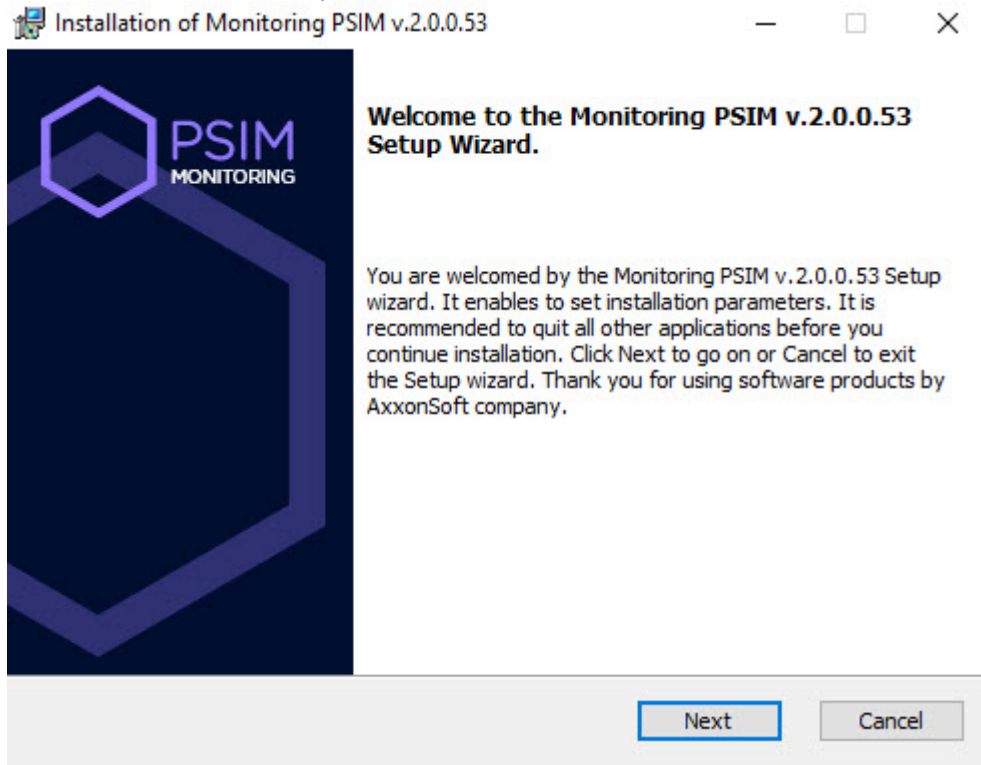


- Read carefully the terms of the license agreement. Then set the switch to the **I accept the terms of the License agreement** position and click the **Next** button.

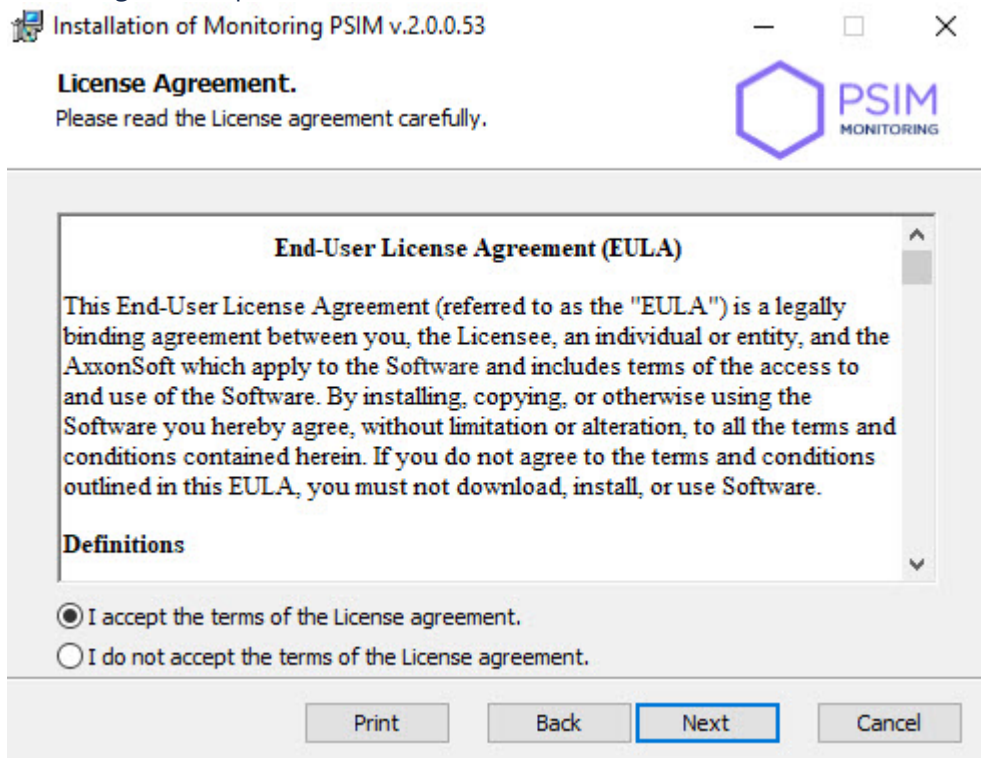

4. Select the **Central server of control** installation type and click the **Next** button.

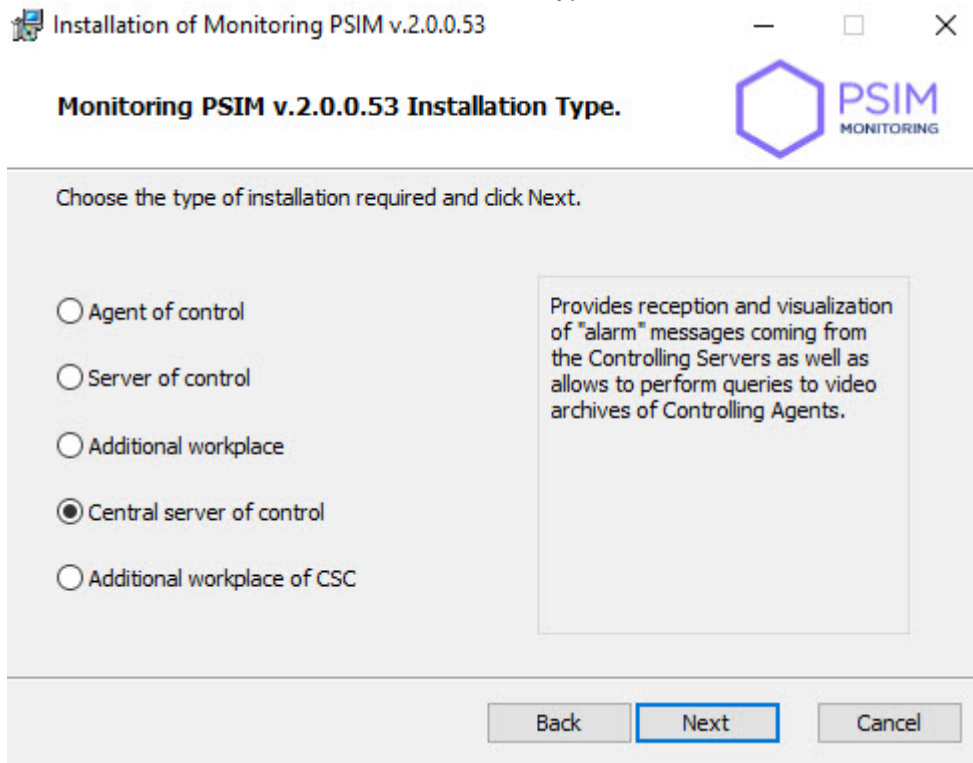

5. If *Axxon PSIM* is installed as a service, and you want to start *Monitoring PSIM* as a service, then set the **Install Monitoring PSIM as a service** checkbox and click the **Next** button (for more details, see [General information about Monitoring PSIM as a service](#)).

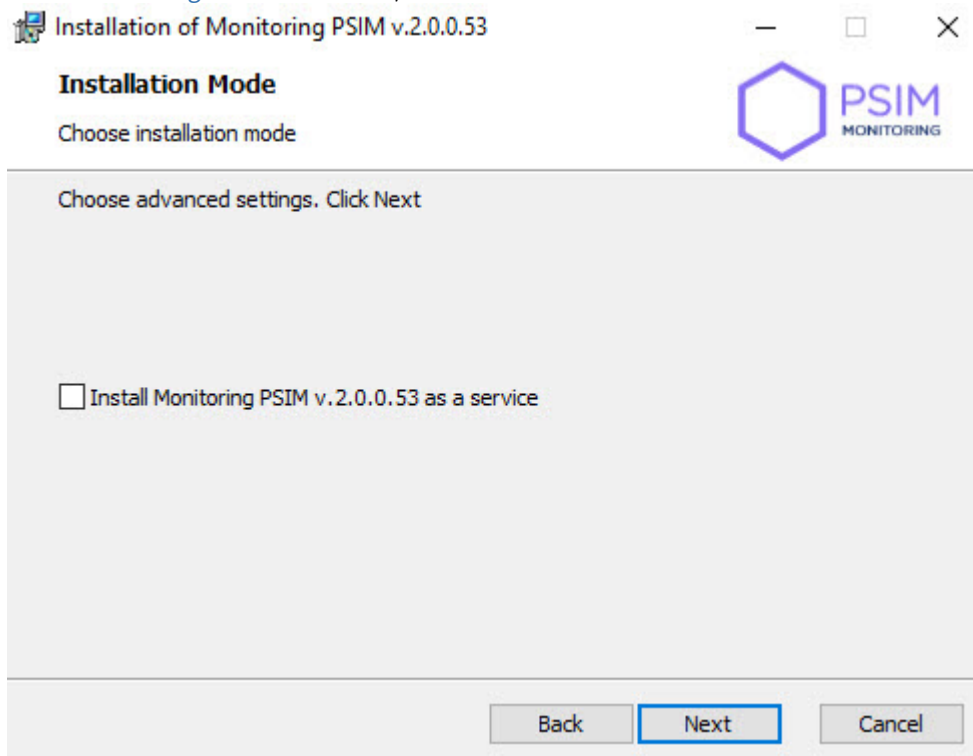

6. Select the MS SQL database server and specify the connection parameters. For more details, see [Installation of Axon PSIM™ software as a Server/Remote administrator workplace](#). To continue the installation process, click the **Next** button.

Note

In the **Select database Server from the drop-down list** field, you must specify the **127.0.0.1** value of the IP address without using the computer names and local value. Otherwise, the *Central server of control* software loses connection with its local database when the network cable is disconnected.

Installation of Monitoring PSIM v.2.0.0.53

Select Database Server

Select database Server and authentication method.

Select database Server from the drop-down list.

127.0.0.1\SQLEXPRESS2014

Choose user identification procedure based on the present user account or SQL Server identity check.

Windows user account

Use the following user name and password:

User name: sa


Password: [Masked]

Back Next Cancel


7. In the **Database** field, specify the name of the database or select it in the list of existing databases from the right and click the << button. Click the **Next** button.

Note


By default, the name of the database is "ServerSSTV" and its files are stored in the SQL Server folder.

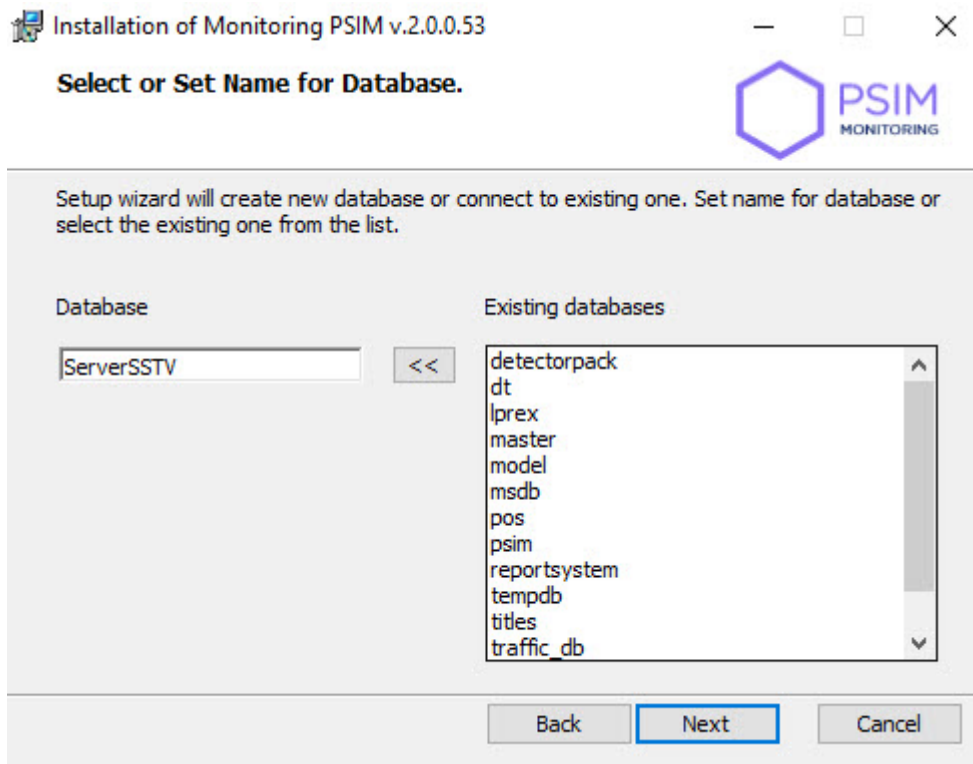


8. Click the **Install** button to start the installation process.

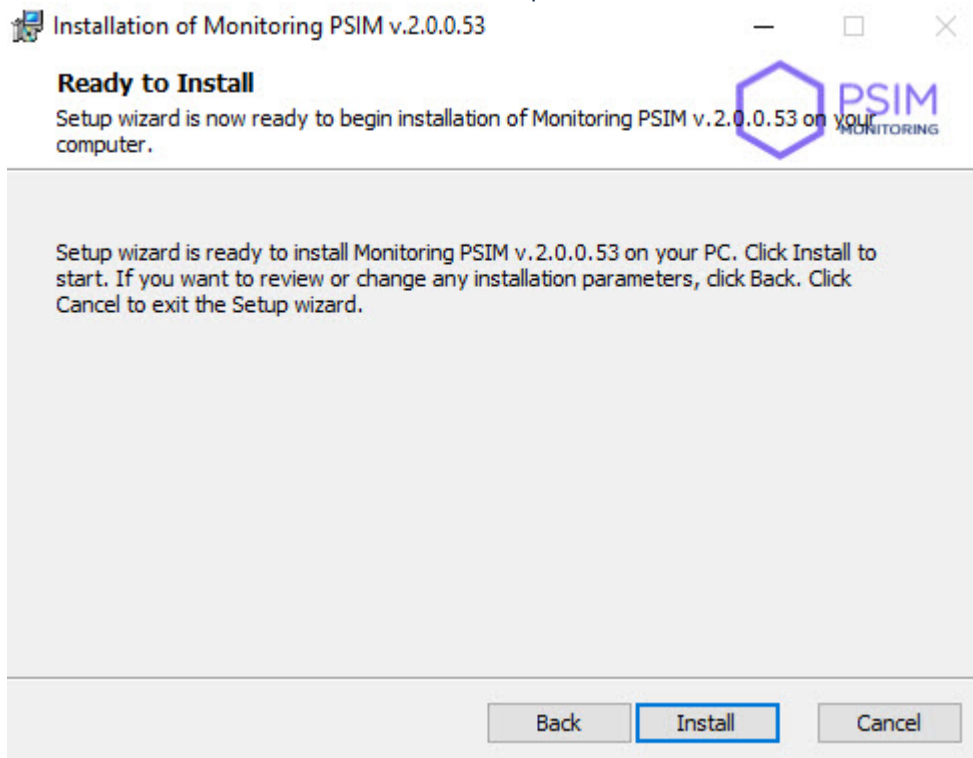

As a result, the system starts copying the required files of *Monitoring PSIM* to the computer's hard disk.

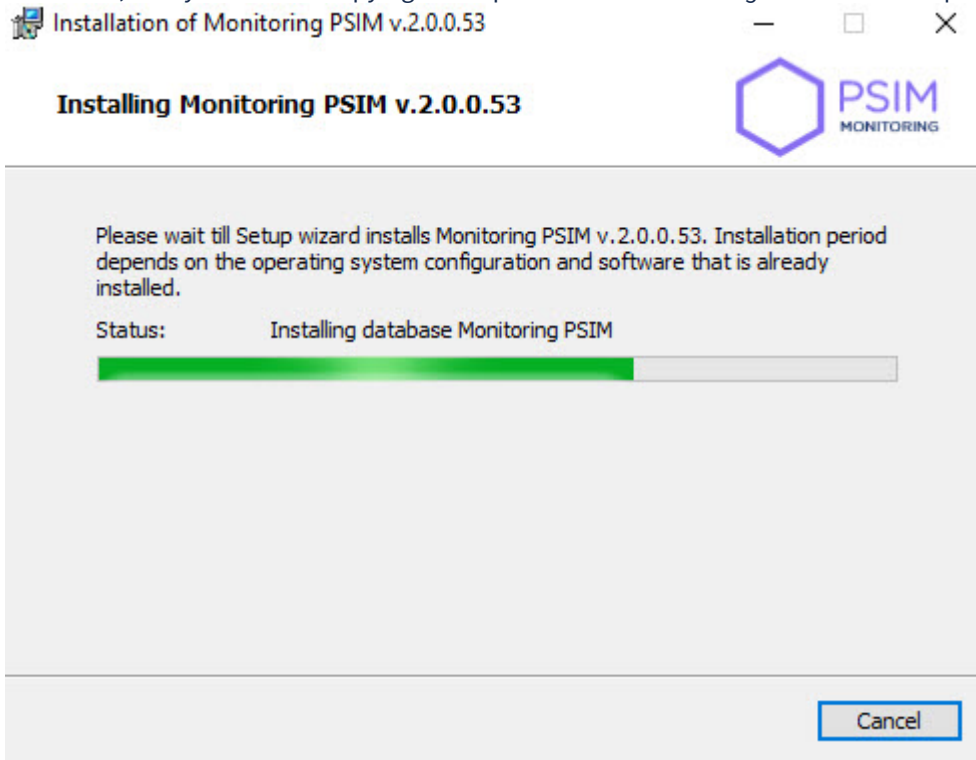

9. After the system successfully copies the *Monitoring PSIM* components, the message about completing the installation process is displayed. Next, click the **Finish** button.

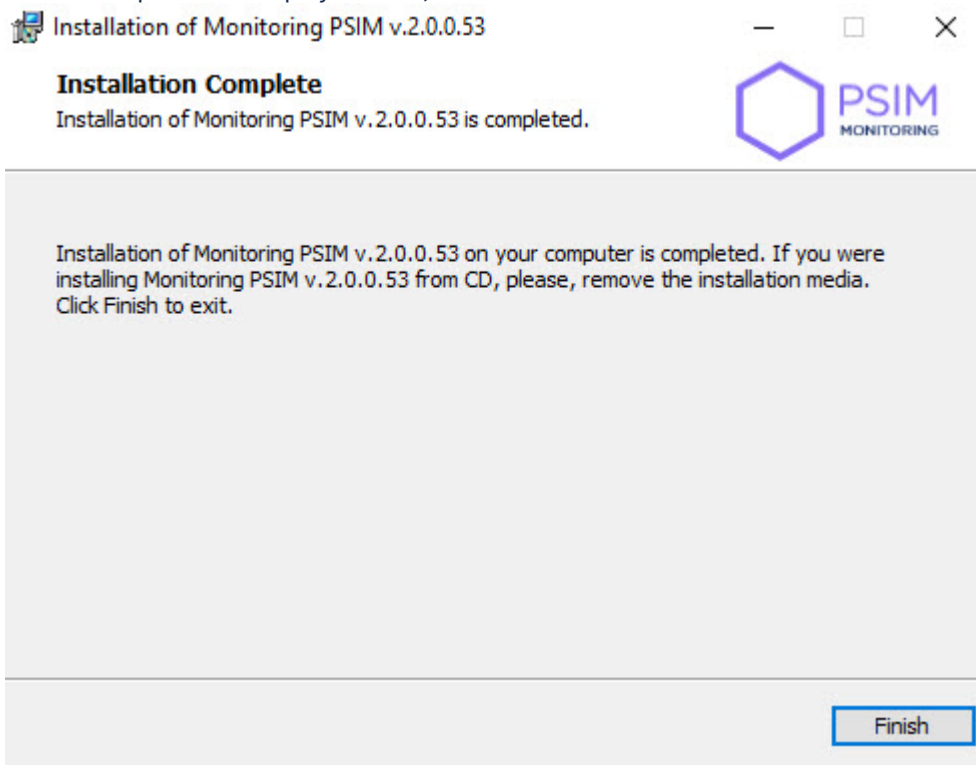


Installing the *Central server of control* software is complete.

4.7 Installing Additional workplace of CSC software


The *Monitoring PSIM* software is installed as a part of the *Axxon PSIM* software. Information about compatibility of the *Axxon PSIM* software versions and *Monitoring PSIM* is presented in the [General information about product releases and versions compatibility](#) section.

To install *Monitoring PSIM* in the *Additional workplace of CSC* software configuration, do the following:


1. In the root directory of the distribution package, run the setup.exe executable file.
2. To continue the installation process, click the **Next** button.

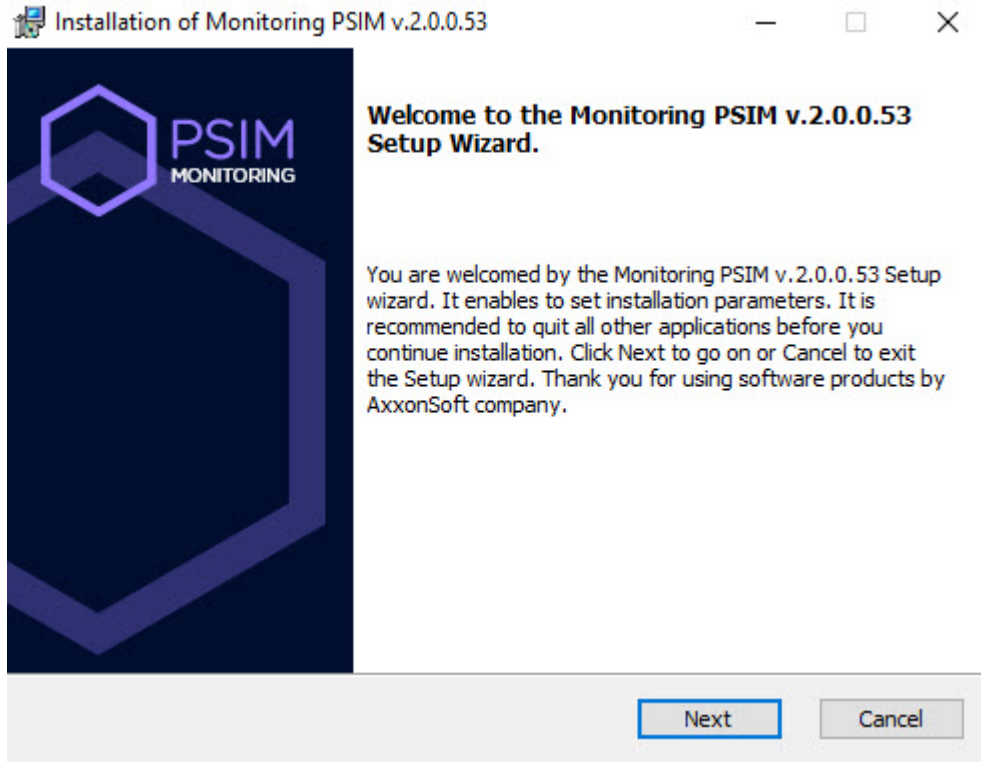

3. Read carefully the terms of the license agreement. Then set the switch to the **I accept the terms of the License agreement** position and click the **Next** button.

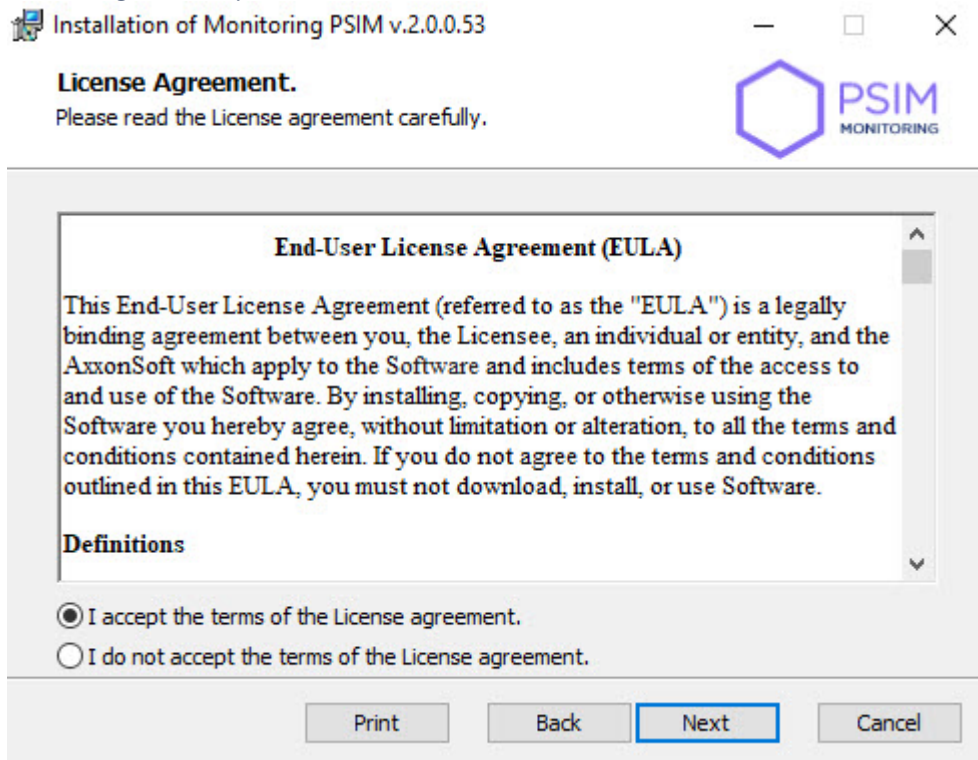


4. Select the **Additional workplace of CSC** installation type and click the **Next** button.

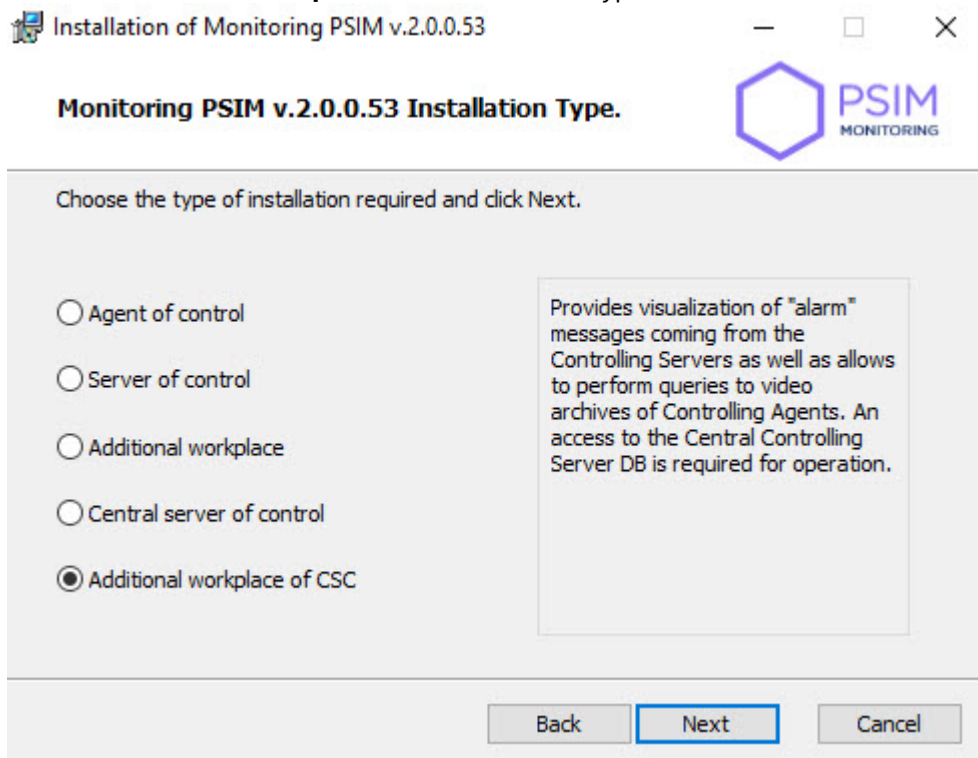

5. Select the MS SQL database server and specify the connection parameters. For more details, see [Installation of Axxon PSIM™ software as a Server/Remote administrator workplace](#). To continue the installation process,

click the **Next** button.

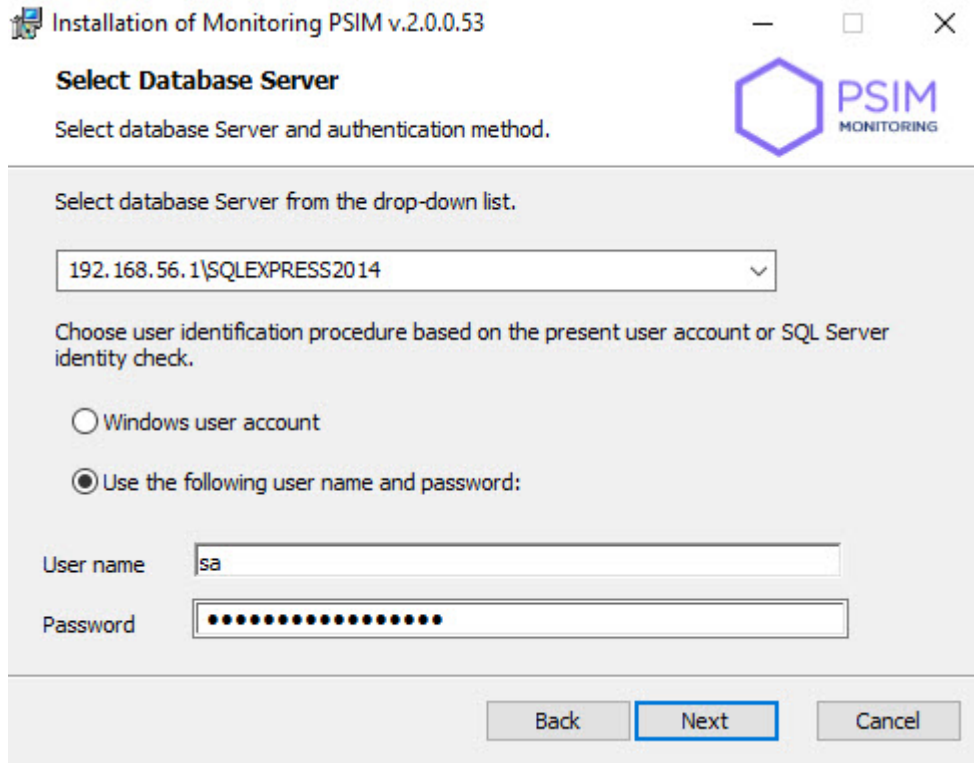

Installation of Monitoring PSIM v.2.0.0.53

Select Database Server

Select database Server and authentication method.

Select database Server from the drop-down list.

192.168.56.1\SQLEXPRESS2014

Choose user identification procedure based on the present user account or SQL Server identity check.

Windows user account

Use the following user name and password:

User name: sa


Password: [Masked]

Back Next Cancel


6. In the **Database** field, specify the name of the database or select it in the list of existing databases from the right and click the << button. Click the **Next** button.

Note

By default, the name of the database is "ServerSSTV" and its files are stored in the SQL Server folder.

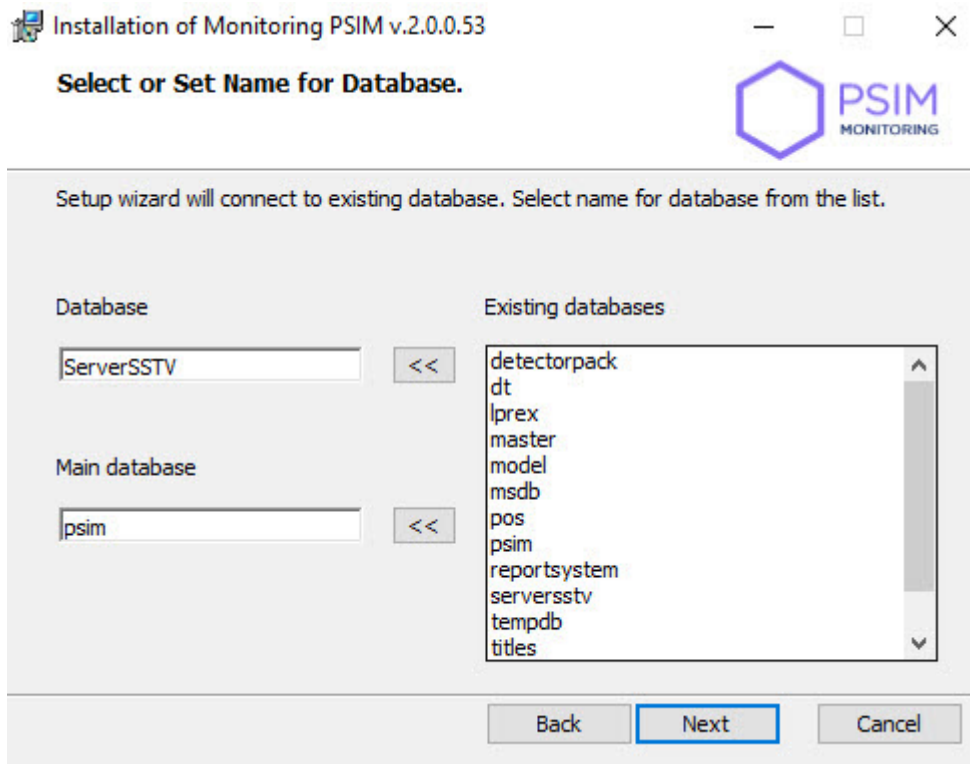

- Specify the export catalog path. This catalog will contain video data received from *Agent of Control*. Click the **Next** button.

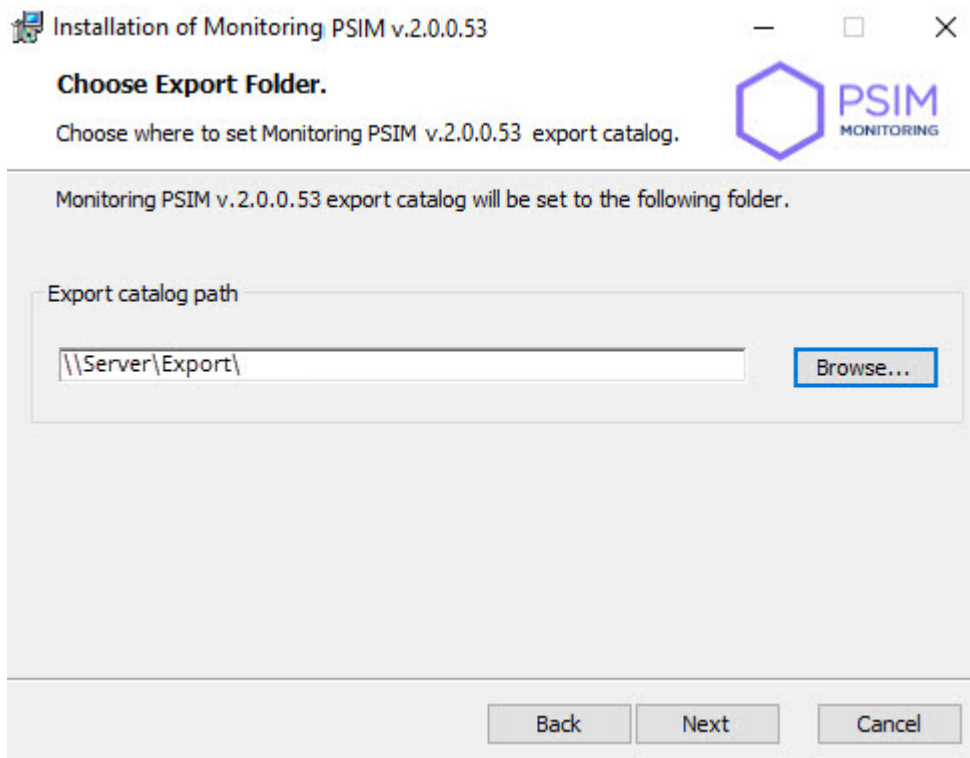

- Specify the IP address and port to connect to the CentralNetServer *Central Server of Control* communication module. Click the **Next** button.


Note

We highly recommend changing the default values for the **Export catalog path** and **IP address** parameters on steps 7-8. Otherwise, after the installation is completed, you must configure *Additional Workplace of CSC* (see [Configuring Additional workplace](#) and [Additional workplace of CSC](#)).

Installation of Monitoring PSIM v.2.0.0.53

Setting up connection to communication module.

Please input ip address and port.



Connection to communication module would be set according to the following values.


Videosrv settings

IP address


Port

Back Next Cancel


9. Click the **Install** button to start the installation process.

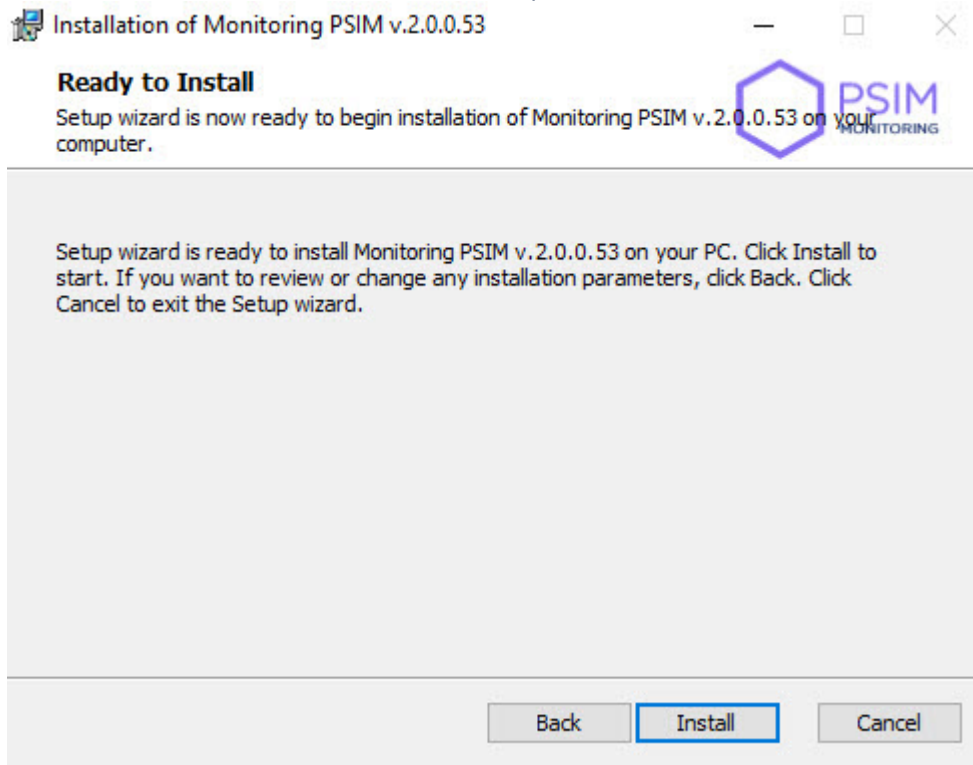

As a result, the system starts copying the required files of *Monitoring PSIM* to the computer's hard disk.

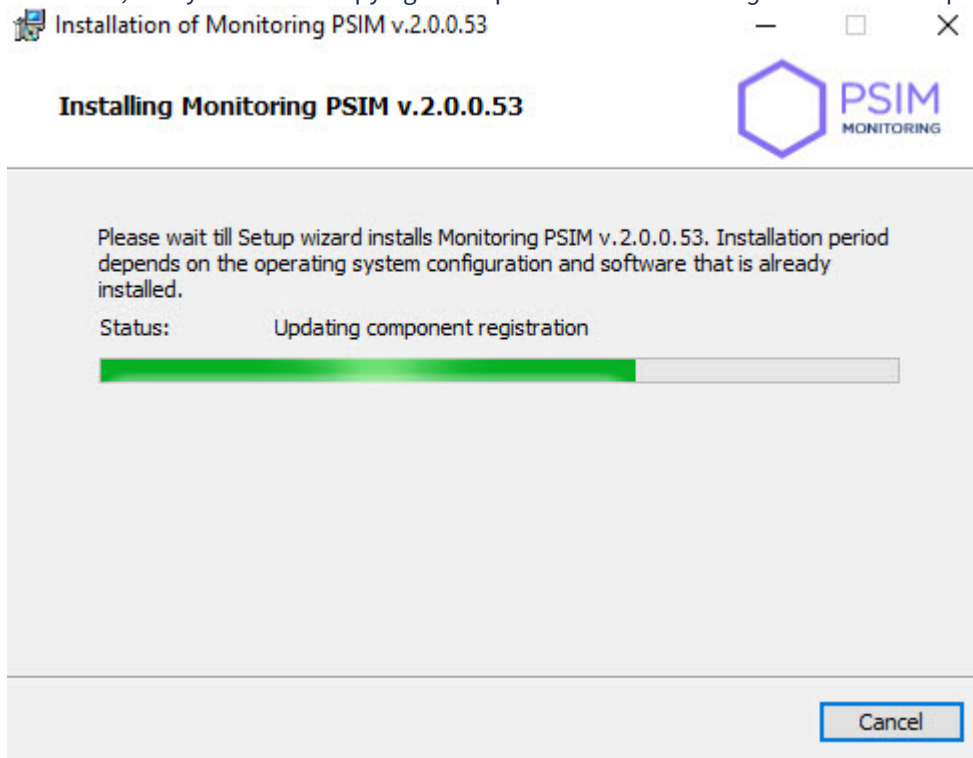

10. After the system successfully copies the *Monitoring PSIM* components, the message about completing the installation process is displayed. Next, click the **Finish** button.

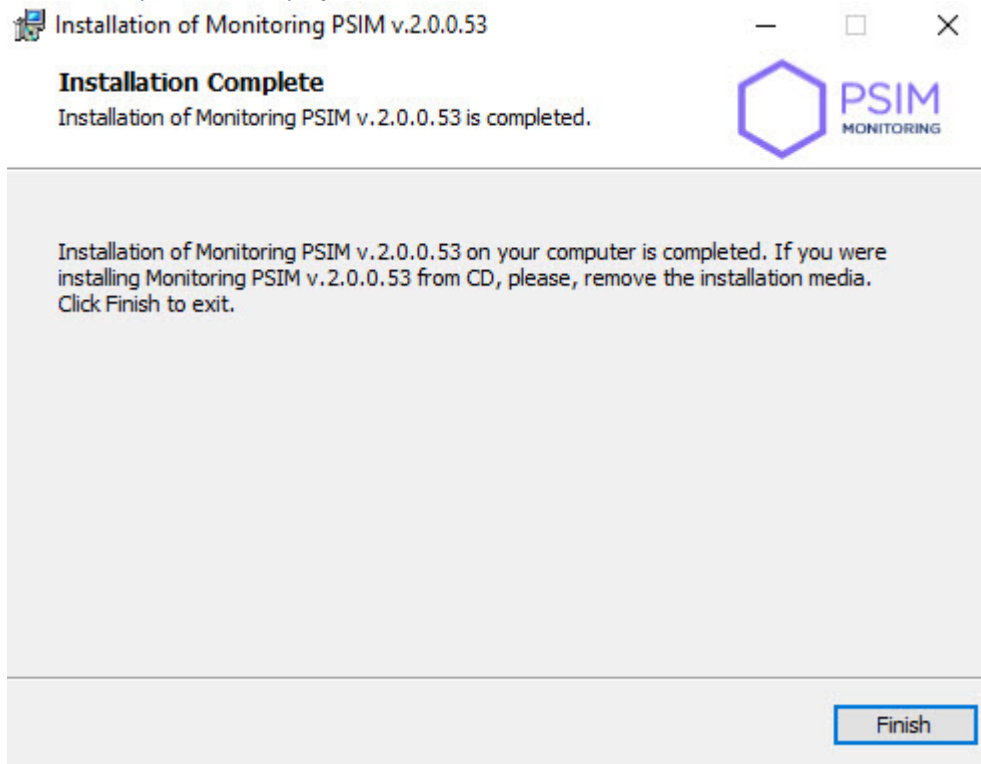

Installing the *Additional workplace of CSC* software is complete.


4.8 Repairing Monitoring PSIM

The repair mode is required to reinstall all components of *Monitoring PSIM*.


To repair *Monitoring PSIM*, do the following:

1. Run the setup.exe executable file in the root distribution directory.


2. Select the **Repair** operation type and click the **Next** button to start the process of repairing.

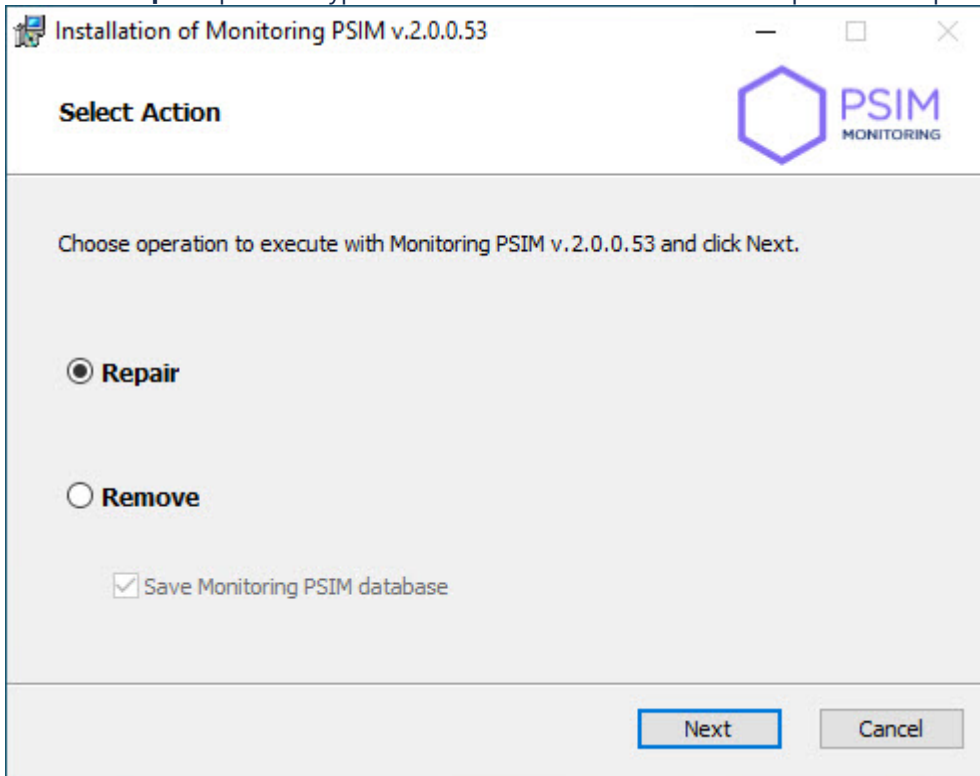

As a result, the system launches a checkup of the installed components and starts copying the required files of *Monitoring PSIM* to the computer's hard disk.

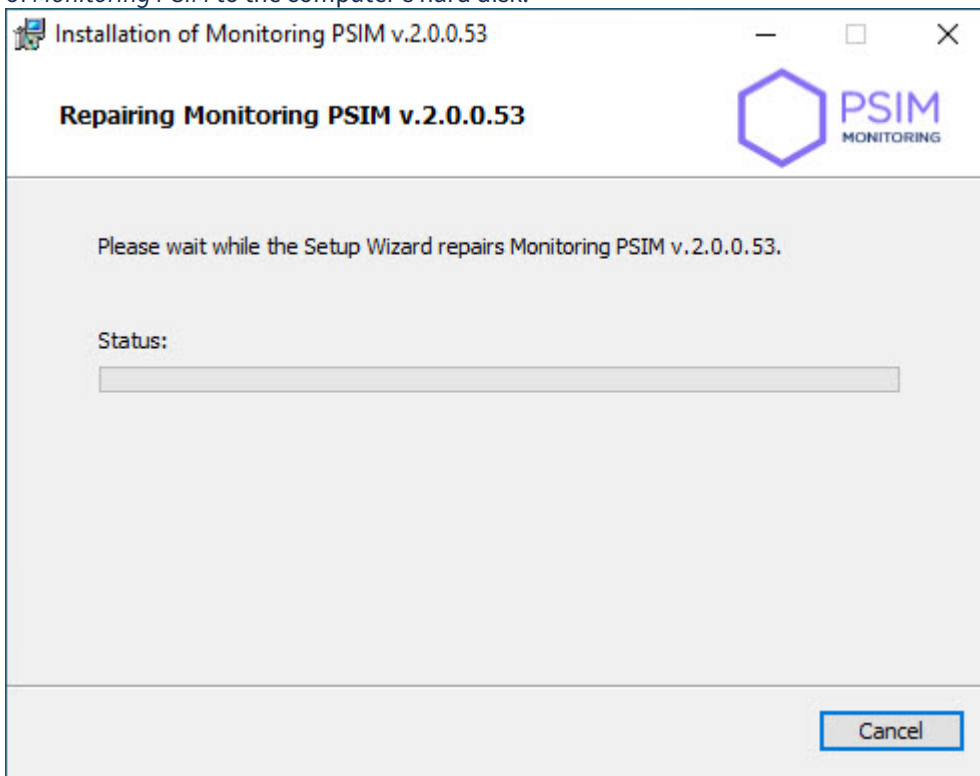

3. After the system successfully copies the *Monitoring PSIM* components, the message about completing the repair process is displayed. Next, click the **Finish** button.

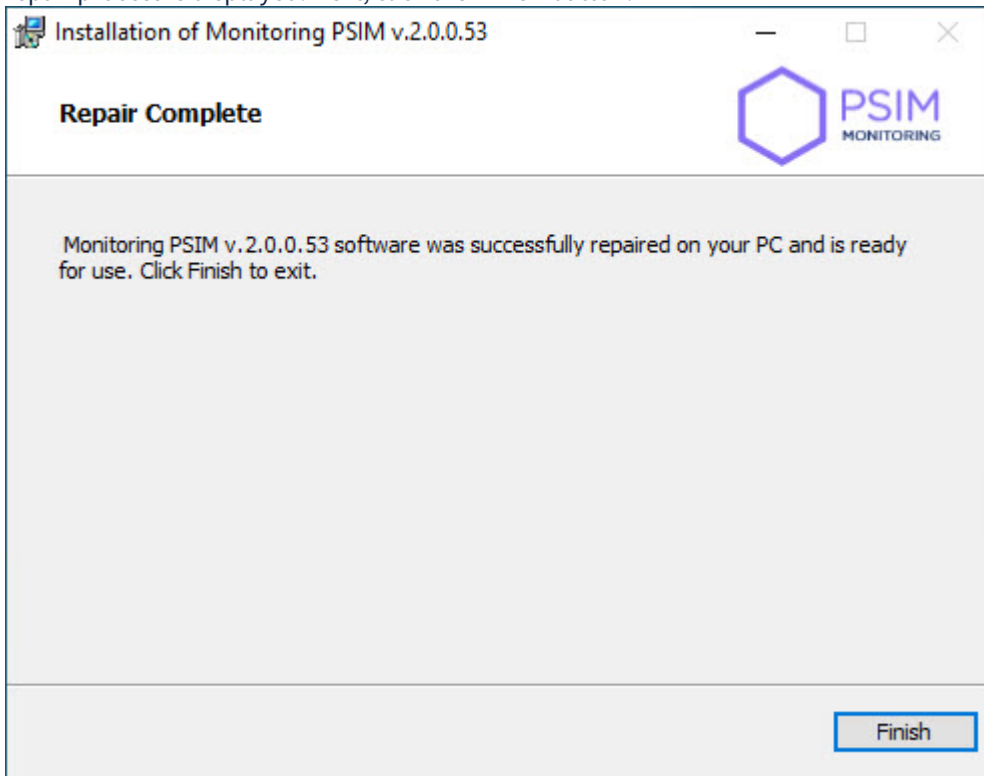

Repairing *Monitoring PSIM* is complete.


4.9 Removing Monitoring PSIM

To remove *Monitoring PSIM*, do the following:


1. Run the `setup.exe` executable file in the root distribution directory.
2. Select the **Remove** operation type and click the **Next** button to start the process of removal.

Note


If you want to save the *Monitoring PSIM* database, set the **Save Monitoring PSIM database** checkbox.

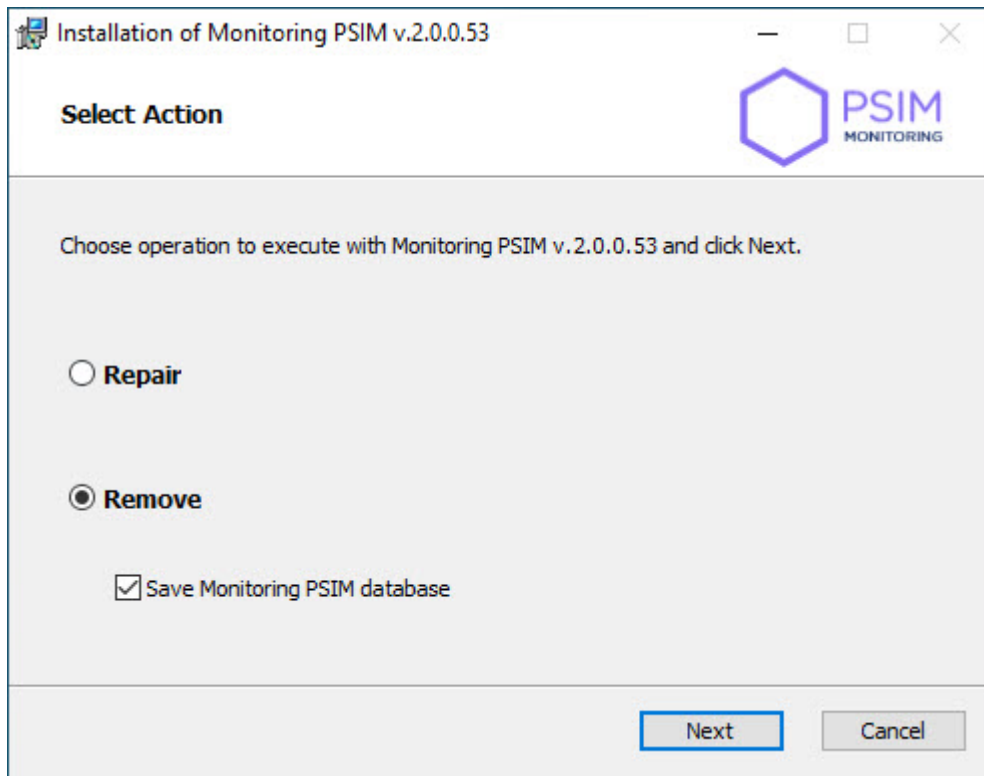

As a result, the system starts removing the installed components of *Monitoring PSIM* from the computer's hard disk.

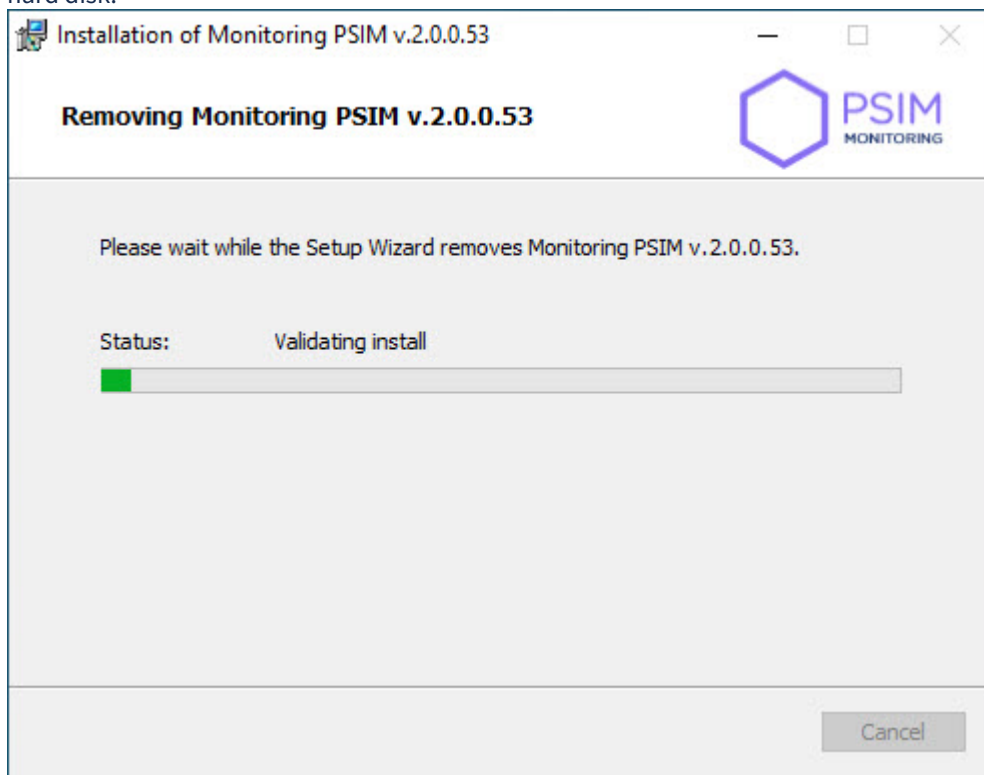

3. After the system successfully removes the *Monitoring PSIM* components, the message about completing the removal process is displayed. Next, click the **Finish** button.

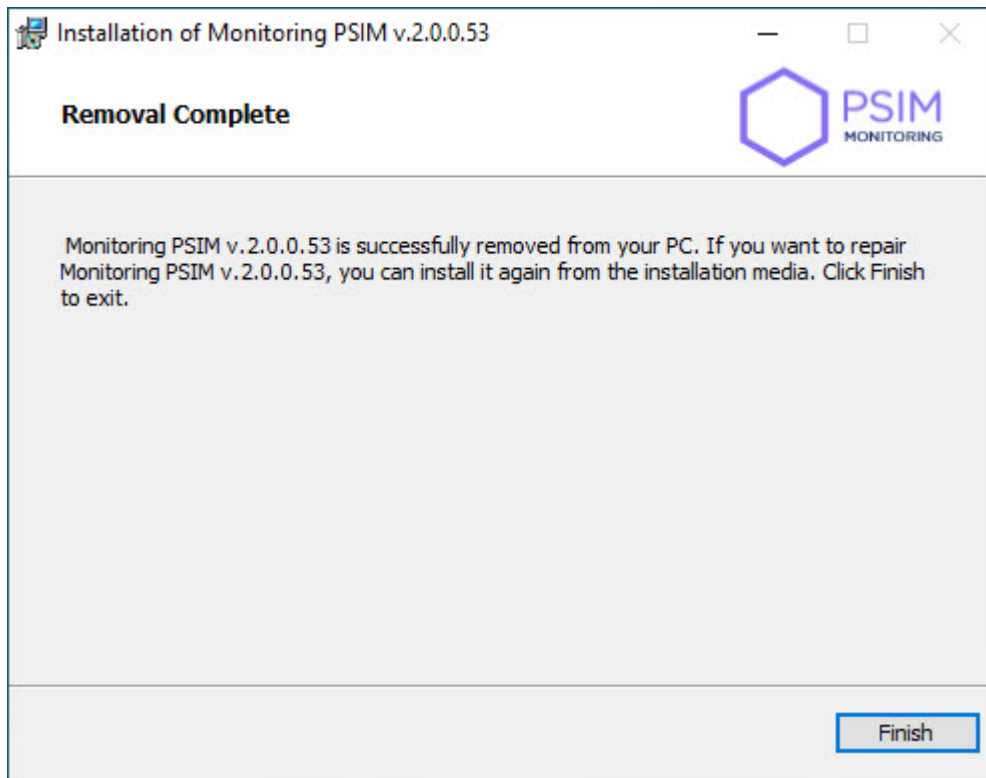

Removing *Monitoring PSIM* is complete.

5 Configuring Agent of Control

To configure *Agent of Control*, go to the **System settings** window. Use of this window is described in [Axxon PSIM Software Package: Administrator's Guide](#).

5.1 Creating necessary Agent Of Control objects

⚠ Attention!


Every time *Agent Of Control* is started, it checks for a **Backup** folder at the root of the disk on which *Axxon PSIM* is installed. If this folder is missing, *Agent Of Control* creates it. It is forbidden to delete this folder.

ℹ Note


Agent Of Control, like *Server Of Control*, can operate in a distributed configuration, at the same time *Agents Of Control*, *Servers Of Control* and *Central Servers Of Control* can see where each of them is installed and can be configured.

To create necessary *Agent of Control* objects, do the following:

1. In the **System settings** dialog window, go to the **Hardware** tab.
2. Create an **IIDK Interface** object based on the **Computer** object. Set the identifier of the **IIDK Interface** object (1).

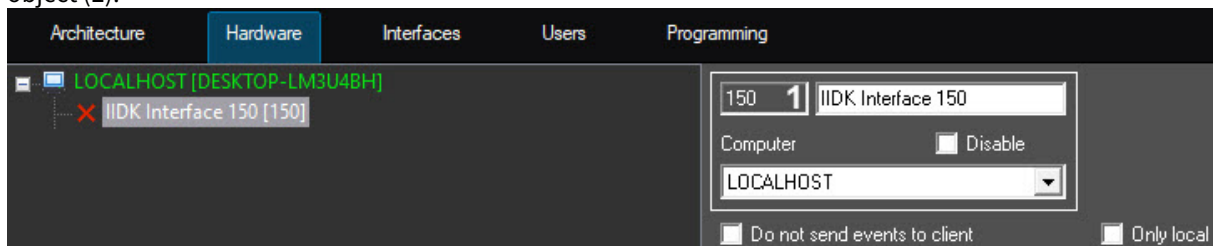


3. Create an **Agent Of Control** object based on the **Computer** object. On the settings panel of this object, in the **IIDK interface** field (2), enter the identifier of the previously created **IIDK Interface** object.

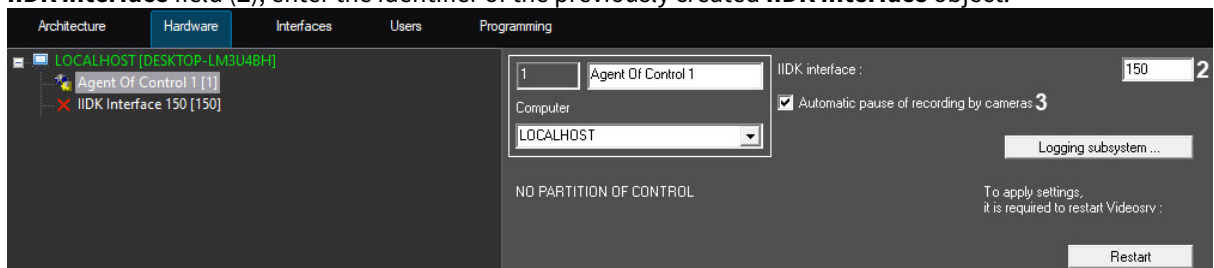

4. The **Automatic pause of recording by cameras** checkbox (3) is set by default, so that the scripts from the code are executed automatically. The **SleepAfterDisarm** and **SleepAfterRecStop** registry keys are used for fine-tuning these scripts (for the description of the registry keys, see [Registry keys reference guide](#)). When the checkbox is clear, you can use the scripts described [here](#) to pause recording by cameras.

5. Create one or more **Partition Of Control** child objects based on the **Agent Of Control** object.

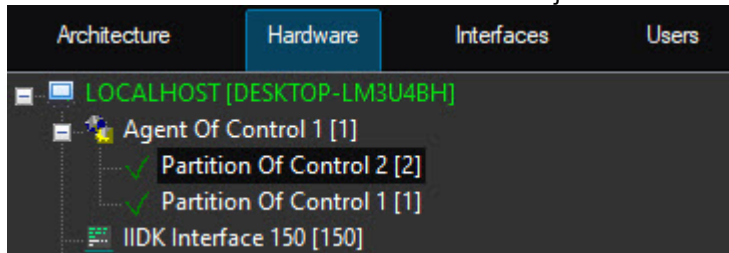

Note

The **Partition Of Control** object name cannot contain the following characters: underscore "_", backslash "\", angle brackets ">" and "<", single quote "'".

It is also necessary to create **Video capture device**, **Camera**, and **Sensor** objects in the hardware tree that correspond to the connected hardware. Creation and configuration of these objects is described in [Axxon PSIM Software Package. Installing and configuring security system components guide](#).


Creation of the necessary objects in the hardware tree is now complete.

5.2 Configuring the logging subsystem

The logging subsystem allows configuring the detail level at which the activity of *Agent of Control* is recorded.

To configure the logging subsystem:

1. Go to the configuration panel for an **Agent Of Control** object.

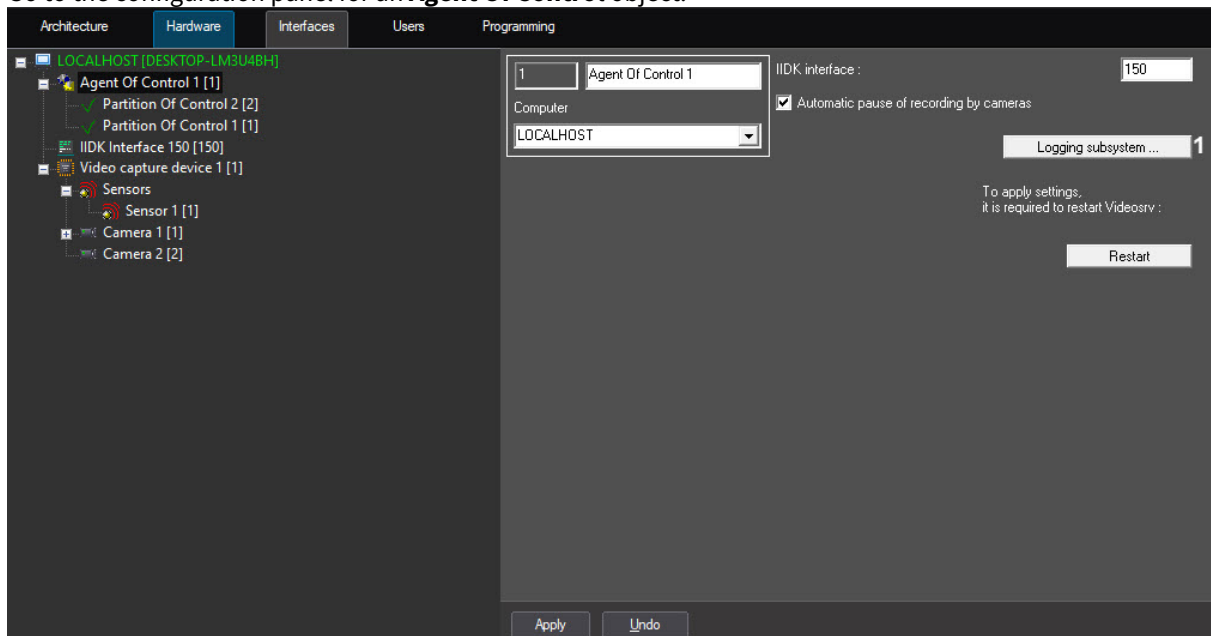

2. Click the **Logging subsystem...** button (1).

3. In the dialog box that opens, specify the following parameters:

- a. **Auxiliary characters:** to log transport-level auxiliary characters, select this check box.
- b. **Alarm events:** to log alarms (activation of vibration sensor, temperature sensor, or forcible entry sensor), select this check box.
- c. **System status:** to log events related to the system state, select this check box.
- d. **Core messages:** to log messages from *Axxon PSIM*, select this check box. Information is saved in the folder to which the software was installed, in the file `video.log`.
- e. **Archiving period (h):** allows archiving the log file at the specified interval (in hours). Archives are saved in the DATA subfolder, with the following name format: `namelog_yymmddhhmmss.gz`, where
 - i. `namelog` is the name of the log file being archived;
 - ii. `yy` is the year of archive creation;
 - iii. `mm` is the month of archive creation;
 - iv. `dd` is the day of archive creation;
 - v. `hh` is the hour of archive creation;
 - vi. `mm` is the minute of archive creation;
 - vii. `ss` is the second of archive creation.
- f. **File size (MB):** sets the threshold size (in megabytes) for the log file after which the file is archived. This setting overrides the value in the **Archiving period (h)** field.
- g. **Keep archives for (months):** sets the length of time for which to store the log file archive, in months (between 1 and 24). Archives that are older than the specified number of months are deleted.

The main log file is located in the installation folder, in the file `vsrvYYMMDD.log`, where YY is the year, MM the month, and DD the day.

Configuration of the logging subsystem is now complete.

5.3 Configuring the Partition Of Control object

5.3.1 Configuring the Partition Of Control unique ID

To configure the unique ID number for a **Partition Of Control** object:

1. Go to the settings panel of the **Partition Of Control** object.

The screenshot shows the configuration interface for a 'Partition Of Control' object. At the top, there are input fields for 'ID' (containing '1'), 'Agent Of Control' (a dropdown menu with 'Agent Of Control 1' selected), and 'TCP port (UPS)' (containing '8888'). To the right of these fields are three buttons: 'Transmitting ...', 'Monitoring ...', and 'Video data ...'. Below the input fields is a table with columns 'Number' and 'Keep archive for (days)', which is currently empty. To the right of this table is a 'Cameras ...' button. Below the table, it says 'Total cameras: 0'. Underneath is a table with columns 'Sensor ID' and 'Sensor type', which is also empty. To the right of this table is a 'Sensors' panel with 'Add ...', 'Edit ...', and 'Delete' buttons. Further right is a 'Registration' panel with the text 'No connection'. At the bottom of the interface, there are 'Apply' and 'Undo' buttons. A large number '2' is placed above the 'Apply' button.

2. In the **ID** field (**1**), enter a unique number for the object on which *Agent Of Control* is being installed. The number can be from 1 to 9 characters long.

Note

The ID cannot contain the following characters: space " ", underscore "_", backslash "\" and single quote "'.

3. To save settings, click the **Apply** button (**2**).

Configuration of a unique **Partition Of Control** ID number is now complete.

5.3.2 Configuring a port for incoming UPS messages

To configure a port for accepting messages from an uninterrupted power supply unit, do the following:

1. Go to the settings panel of the **Partition Of Control** object.

The screenshot shows the configuration interface for a Partition Of Control object. At the top, there are input fields for 'ID' (386), 'TCP port (UPS)' (8888), and a dropdown for 'Agent Of Control' (Agent Of Control 1). To the right are buttons for 'Transmitting ...', 'Monitoring ...', and 'Video data ...'. Below these is a table for cameras with columns 'Number' and 'Keep archive for (days)'. A 'Cameras ...' button is next to the table, and 'Total cameras: 0' is displayed below. A similar table for sensors is shown below, with 'Sensors: 0' below it. To the right of the sensor table are 'Add ...', 'Edit ...', and 'Delete' buttons. Further right is a 'Registration' panel showing 'No connection'. At the bottom, there are 'Apply' and 'Undo' buttons, with a '2' above the 'Apply' button.

2. In the **TCP port (UPS)** field (1), enter the number of the port on which to "listen" for UPS messages.
3. To save the settings, click the **Apply** button (2).

Configuration of a port for accepting messages from a UPS is now complete.

5.3.3 Configuring communication between Agent Of Control and Server Of Control

Note

Before you configure the interaction between the *Agent Of Control* and the *Server Of Control*, it is recommended to make sure that the name and identifier of the **Partition Of Control** object being configured are specified correctly, since upon the successful connection to the *Server Of Control*, if an object with this identifier is absent, the **Partition Of Control** object with the name and identifier of the object being configured will be automatically created on it. If the interaction between the *Agent Of Control* and the *Server Of Control* is configured successfully, the **Registration completed** message will be displayed in the **Registration** area (1). This means that the *Agent Of Control* can transmit alarms and data on the technical state of this *Partition Of Control* to the *Server Of Control*.

If the **Partition Of Control** object could not be created on the *Server Of Control*, the reason will be indicated in the **Registration** area, for example:

- **The base software is not loaded;**
- **Change the object name** (an object with the same name already exists on the *Server Of Control*);
- An object on the *Server Of Control* will also not be created if the user does not have rights to administer the *Server Of Control* object (see [Rights administration](#)).

To configure the communication between the *Agent Of Control* and the *Server Of Control*, do the following:

1. Go to the settings panel of the **Partition Of Control** object.

1

Partition Of Control 1

ID 386

TCP port (UPS) 8888

Agent Of Control 1

Transmitting ...

Monitoring ...

Video data ...

Number	Keep archive for (days)

Cameras ...

Total cameras: 0

Sensor ID	Sensor type

Sensors

Add ...

Edit ...

Delete

Registration

No connection

Sensors: 0

Apply

Undo

- Click the **Transmitting** button (2). A dialog box opens with settings for configuring the communication method between the *Agent Of Control* and the *Server Of Control*.

- In the **Connection to Control Server** drop-down list, select the **Client mode** as the methods for connecting the *Agent Of Control* to the *Server Of Control* (1).

Note

The **Server mode** is not used.

- From the **Connection** drop-down list, select the value for the transport level. Possible values are **TCP/IP** or **RS232** (2).
- If the **RS232** connection type is selected, then specify the **COM port number**, **COM port speed**, and **COM port format** parameters (3).
- If the **TCP/IP** connection type is selected, then indicate the parameters for connection to the *Server Of Control* in this dialog box:
 - If an IP address is used for connection, make sure that the **Use DNS instead of IP** checkbox is not set (5) and indicate the **IP address** and **TCP port** of the *Server Of Control* (4).

- b. If a domain name is used for connection, set the **Use DNS instead of IP** checkbox (5) and indicate the **DNS name** and **TCP port** of the *Server Of Control*.

The screenshot shows a configuration window titled 'TCP/IP'. It contains the following fields and controls:

- TCP port:** A text input field containing the value '7777'.
- DNS name:** A text input field containing the value 'server.local'.
- Use DNS instead of IP:** A checked checkbox.

Note

The use of domain name for connection allows you to avoid the *Agent Of Control* resetting in case of *Server Of Control* IP address change.

7. When still frames or video is sent to the *Server Of Control*, the data is transferred in packets. The packet size is specified by the **I/O buffer (bytes)** parameter (6). For maximum data transfer speed, it is recommended to use the value 4096. For poor connections, such as if a GSM modem is used, it is recommended to use the value 800.
8. If **Client mode** is selected, in the **Ping frequency (s)** field (7), enter the time interval at which the *Agent Of Control* will send messages about its technical state to the *Server Of Control*. Minimum possible value is 10 sec. This value does not affect short-term alarms. Messages about short-term alarms are transmitted from the *Agent Of Control* to the *Server Of Control* immediately after corresponding sensors triggering. Some long-term alarms can also be an exception: for more information, see [Appendix 1. Data update periods summary](#).
9. Click the **OK** button (8) to save the connection settings and return to the settings panel of the **Partition Of Control** object.
10. Click the **Apply** button to save the changes.

Configuration of communication between the *Agent Of Control* and the *Server Of Control* is now complete.

5.3.4 Configuring captions


To use and configure captions, for each camera on which you want to use captions, you must create a **Captioner** object.

Attention!


If multiple captioners have been created for a single camera, the *Agent Of Control* uses the captioner with the lowest ID number.

To configure the font and display area used for captions, do the following:


1. In the hardware tree, click the relevant **Captioner** object. On the right side of the **System settings** dialog box, the settings panel of the **Captioner** object is displayed.

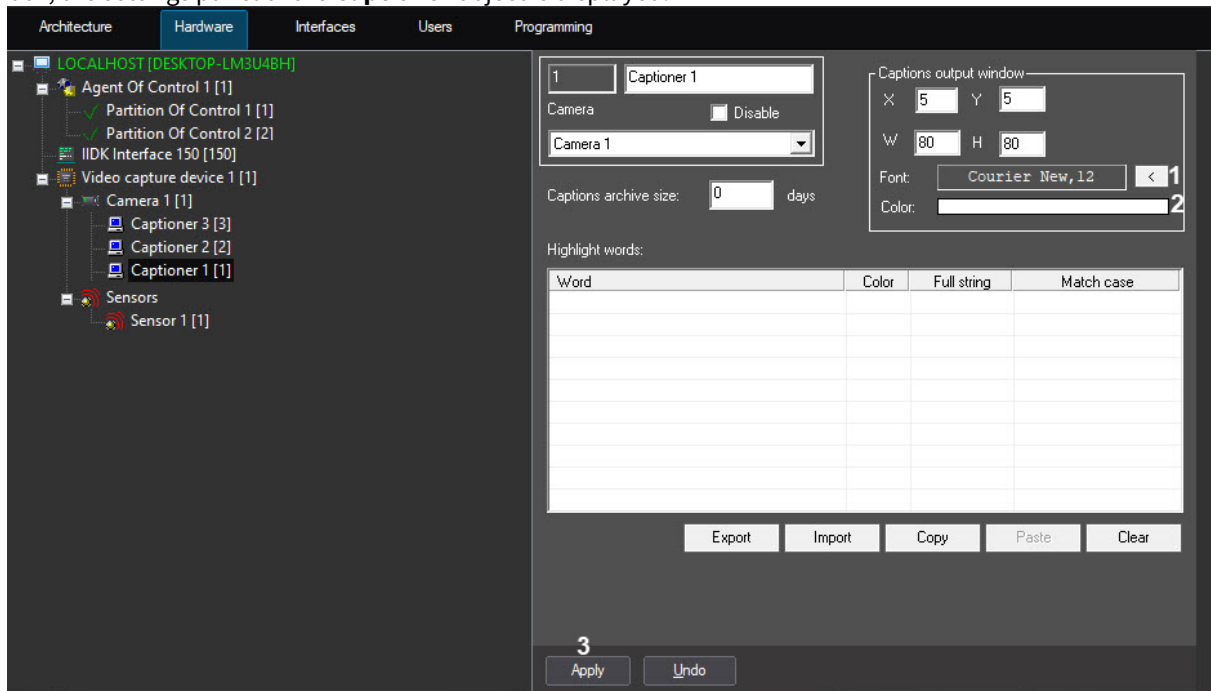

2. If you click the button to the right of **Font**, a dialog box appears in which you can configure the font face and size (1).

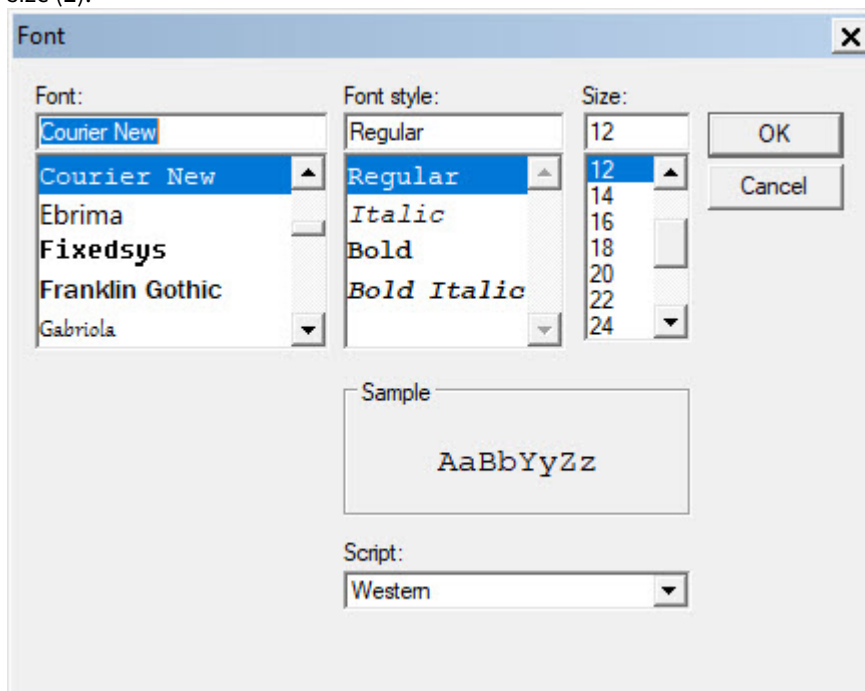

- To configure the color of captions, double-click the area to the right of **Color**. A dialog box for configuring color appears (2).

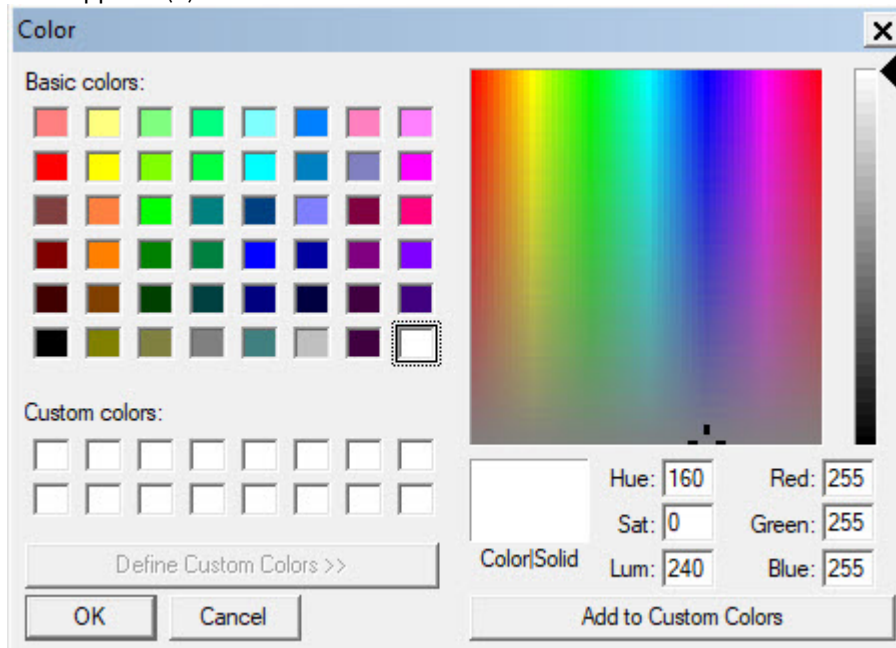

Configuration of the **Captioner** object is now complete.

5.3.5 Configuring the camera list

The list of cameras specified in the configuration panel for the **Partition Of Control** object determines the cameras whose archive and video can be accessed through the *Monitoring PSIM* interface objects (see [Monitoring PSIM Software Package: Operator's Guide](#)). In addition, this list determines the cameras whose state and archives are monitored by *Agent of Control*.

Depending on whether the list of cameras has been specified or not, the following situations are possible:

- If cameras are specified in the list, *Agent of Control* works in normal mode: it monitors the state of cameras and their archives. *Server of Control* receives information about the number of cameras, disks, disk volume, etc.
- If no cameras are specified in the list, *Agent of Control* checks the presence of a **Backup archive** object in the system and gets information about disks from this object. In this case, *Server of Control* will receive information only about the disks marked in the **Backup archive** object. Access to the archive is not performed from the **Search in archive** interface object during this process.
- If no cameras are specified in *Agent of Control* settings and there is no **Backup archive** object in the configuration, information about disks is taken from the **Computer** object; the disks specified for storage of the main archive are taken into account. Access to the archive is not performed from the **Search in archive** interface object during this process.

In the second and third cases, monitoring is performed of the state of the system (network functioning, restarts, etc.) and disks (their number and free space). The state of cameras and their archives is not available for monitoring.

Note


Creation and configuration of the **Backup archive** object is described in [Axxon PSIM Software Package: Administrator's Guide](#).



To configure the list of cameras in use, do the following:

1. Go to the settings panel for the **Partition Of Control** object.

The screenshot shows the configuration interface for a 'Partition Of Control' object. At the top, there are input fields for 'ID' (386), 'TCP port (JPS)' (8888), and a dropdown for 'Agent Of Control' (Agent Of Control 1). To the right are buttons for 'Transmitting ...', 'Monitoring ...', and 'Video data ...'. Below these is a table with columns 'Number' and 'Keep archive for (days)'. A 'Cameras ...' button with a count of '1' is positioned to the right of the table. Below the table, it says 'Total cameras: 0'. Underneath is a table with columns 'Sensor ID' and 'Sensor type'. To the right of this table are buttons for 'Add ...', 'Edit ...', and 'Delete'. Further right is a 'Registration' box containing the text 'No connection'. Below the sensor table, it says 'Sensors: 0'. At the bottom of the panel are 'Apply' and 'Undo' buttons.

- Click the **Cameras...** button (1). The **Add/Edit cameras** window opens.

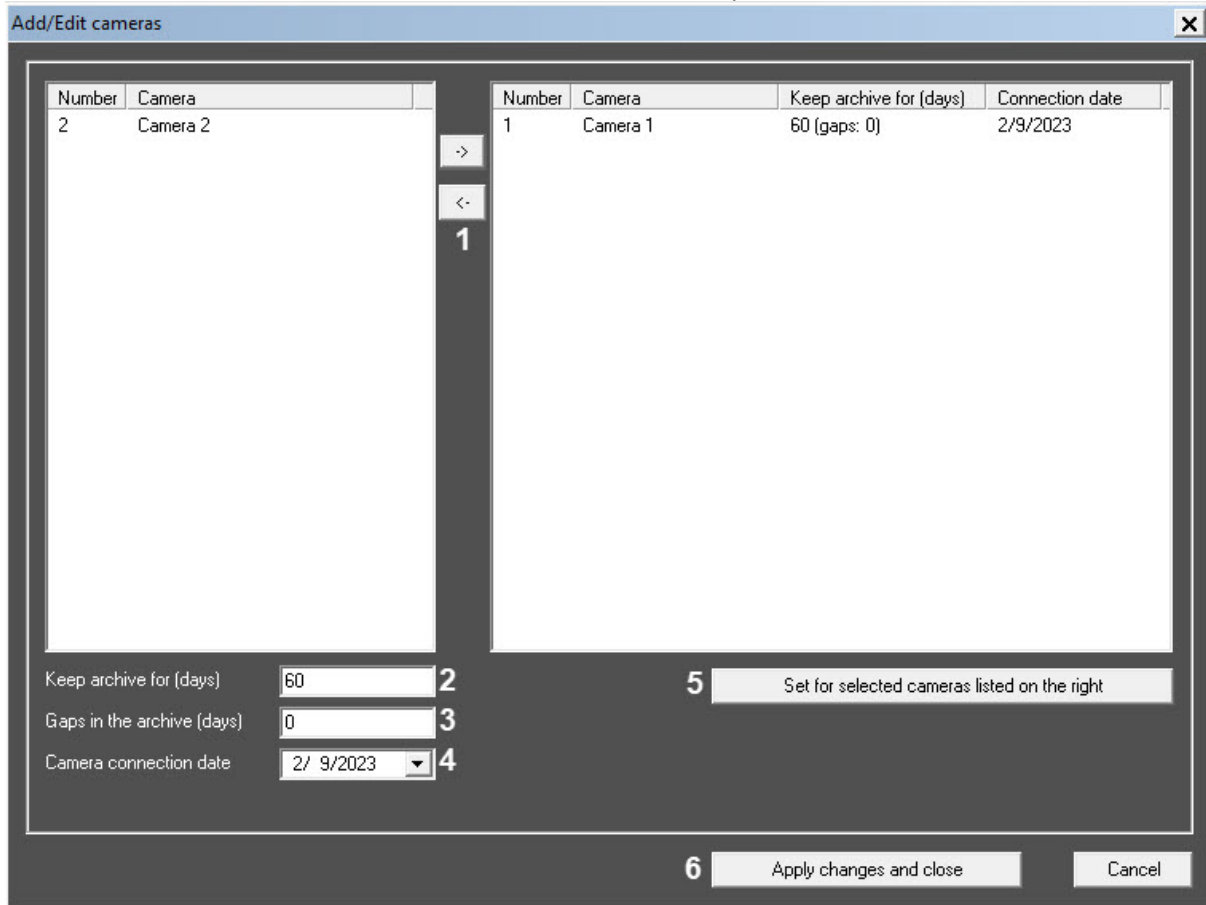

- Move the necessary cameras from the left list to the right list by clicking the  and  buttons (1).
- Select cameras in the list on the right.
- In the **Keep archive for (days)** field, specify the storage time of the video archive in days (2) in the range from 0 to 999. If the value of the parameter is 0, the size of the archive will not be monitored.
- In the **Gaps in the archive (days)** field, specify the number of days on which the video archive is not recorded, because non-working days are taken into account in the working schedule (3).
- In the **Camera connection date** field, specify the date the camera was connected to the system (4).
- Click the **Set for selected cameras listed on the right** button (5).
- Click the **Apply changes and close** button (6). The selected cameras will be added to the list on the settings panel of the **Partition Of Control** object.
- Click the **Apply** button on the settings panel of the **Partition Of Control** object.

Note

The ID numbers of cameras and captioners must be whole numbers.

Note

Cameras will be automatically removed from the list in the following cases:

- The **Camera** object or its **Video capture device** parent object is removed from the *Axxon PSIM* hardware list;

- The **Camera** object or its **Video capture device** parent object is set to **Disabled** mode;
- In a distributed configuration, the **Camera** object is moved to a **Video capture device** object located on another computer;
- In a distributed configuration, the **Video capture device** object, to which the **Camera** object belongs, is moved to another computer.

Configuration of the camera list is now complete.

5.3.6 Configuring sensors

The system supports use of four fixed sensors (vibration sensor, lock sensor, temperature sensor, and additional sensor) as well as 12 expansion sensors.

 **Note.**

Before configuring a list of sensors for a protected site, you must create and configure the necessary **Sensor** objects in *Axxon PSIM* first. Creation and configuration of these objects is described in the document [Installing and configuring security system components guide](#).

 **Attention!**

Sensor IDs must be whole numbers.

 **Note**

If video data (i.e. clips or snapshots) are attached to the alarms, it is necessary to create a script for stopping recording on camera (see [Sample script for stopping camera recording](#)).

To configure the list of sensors in use:

1. Go to the configuration panel for the **Partition Of Control** object.

1 Partition Of Control 1 ID 386 Transmitting ...

Agent Of Control 1 TCP port (UPS) 8888 Monitoring ...

Video data ...

Number	Keep archive for (days)
--------	-------------------------

Cameras ...

Total cameras: 0

Sensor ID	Sensor type
-----------	-------------

Sensors: 0

Sensors

- Add ... 1
- Edit ...
- Delete

Registration

No connection

Apply Undo

- Click the **Add** button (1). A dialog box for adding a sensor appears.

The dialog box contains the following fields and options:

- Type: 1 Vibration sensor
- Name: 2 VIBROSENSOR
- ID: 3 Sensor 1 [1]
- Assignment to camera: 4 Camera 1 [1]
- 5 Transmit snapshots
- 6 Transmit video
- 7 Post-alarm time (s): 20
- 8 Pre-alarm time (s): 0
- 9 Number of frames: 1
- 10 Interval (s): 1
- Captioning 11
- Show for (s): 5 12
- 13 OK
- Cancel

- In the **Type** drop-down list, select the type of sensor from the sixteen types described previously (1).
- In the **Name** field (2), enter the text that will be sent to *Server of Control* together with the alarm message. This text will be overlaid on the video during the captioning process.
- In the **ID** drop-down list, select a **Sensor** object that has been previously created in the *Axxon PSIM* device tree (3).
- In the **Assignment to camera** drop-down list, select a video camera from which the video frames or video clips should be requested (4).
- To enable sending video frames to *Server of Control* when a sensor is activated, select the **Transmit snapshots** check box (5).
- If you want for a video fragment to be sent to *Server of Control* when a sensor is triggered, select the **Transmit video** check box (6).
- In the **Post-alarm time (s)** field, enter the time delay between when a sensor is triggered and the time of access to the video archives, in seconds (7). The default value is 20 seconds. This parameter is necessary for guaranteed recording on camera.
- In the **Pre-alarm time (s)** field, specify the amount of time for which you want to pre-record before sensor triggering, in seconds (8). This allows obtaining video frames depicting not only the very moment at which an alarm occurs, but a short time before.
- If the **Transmit snapshots** check box was selected:
 - In the **Number of frames** drop-down list, select the quantity of video frames to be transferred when a sensor is triggered (9).
 - In the **Interval (s)** field, enter the length of time, in seconds, between video frames if more than one frame is to be sent (10). Thus when an alarm occurs, it is possible to send to *Server of Control* an


entire sequence of frames that represent different points in time, which increases the chance of viewing the most valuable frames.

⚠ Attention!

For snapshots transmitting more, as well as for video clips transmitting, it is necessary to create a script for stopping video recording on camera (see [Sample script for stopping camera recording](#)).

⚠ Attention!

When specifying the **Pre-alarm time (s)**, **Number of frames**, and **Interval (s)** settings, keep an eye on the configuration of the camera from which video frames are to be sent, and particularly on the **Pre-alarm record... (s)** setting. **Pre-alarm record... (s)** time on camera have to be greater or equal to **Pre-alarm time (s)** value in sensor settings.

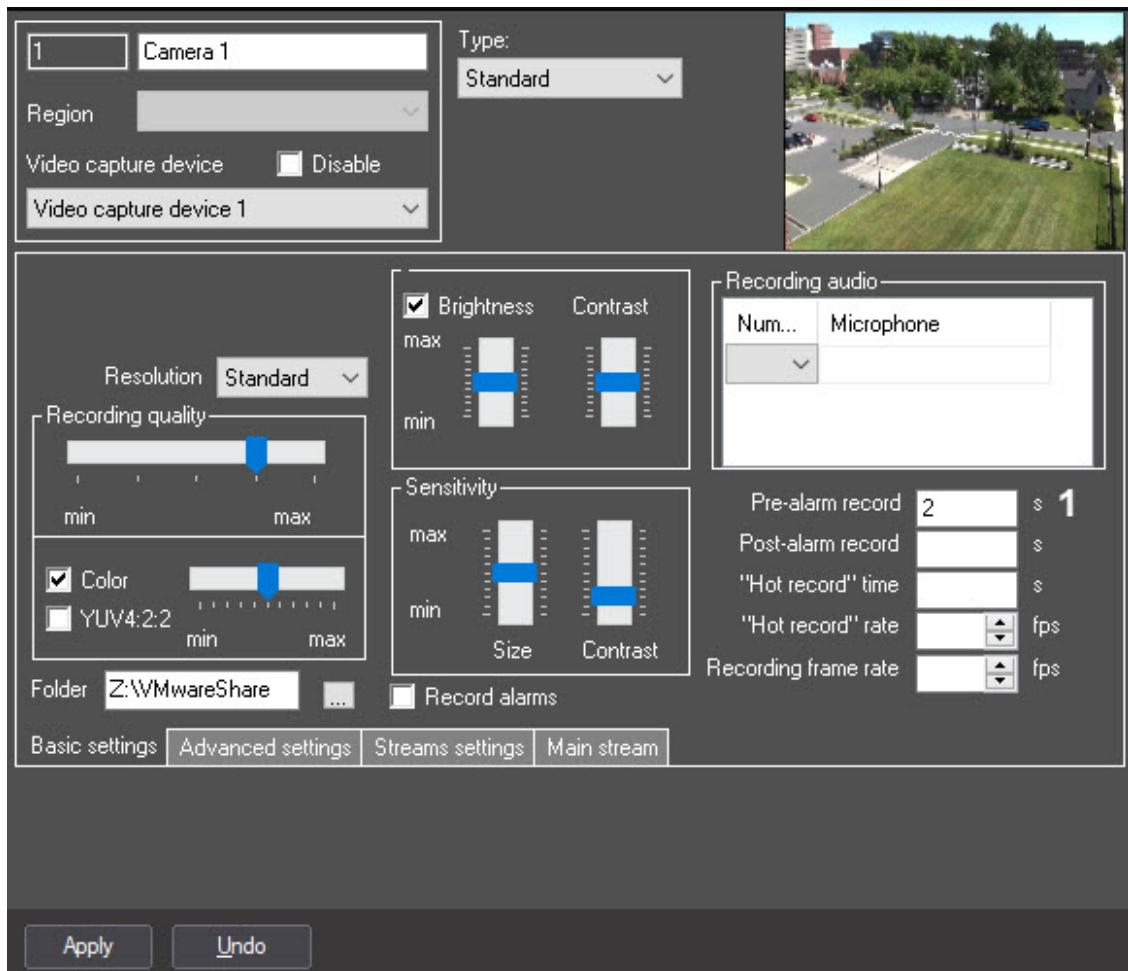

12. If the **Transmit video** check box (1) was selected:
 - a. In the **Length (s)** field (2), specify the length of the video fragment to send.

⚠ Attention!

If the **Not used** value is selected in the **Export to avi** parameter (3), then the **Length (s)** parameter will be unavailable. In this case, the length will be determined by the size of the video fragment file in the video archive. To limit the length of the video fragment to be sent, use a script to stop recording on the camera (a sample script is found in the [Sample script for stopping camera recording](#)).

- b. In the **Rate (Kbyte/s)** field, enter the transmission rate for the video fragment (3).
- c. The **Export to avi** parameter (4) allows you to select the format and codec of the requested video clip:
 - **Not used** – the video clip will be exported as an archive with a set of directories and files from the VIDEO folder.
 - **Initial format** – the video clip will be exported to an AVI-file without transcoding,
 - **Xvid** – the video clip will be exported to an AVI-file with the Xvid codec,
 - **DivX** – the video clip will be exported to an AVI-file with the DivX codec,
 - **x264** – the video clip will be exported to an AVI-file with the x264 codec.
13. If it is necessary to overlay captions on video when a sensor is triggered, select the **Captioning** check box (11). In the **Assignment to camera** field, specify the camera on whose video you want to overlay captions (4).
14. In the **Show for (s)** drop-down list, select the amount of time for which you want captions to be displayed on video, in seconds (12).
15. Click **OK** (13).


Configuration of the list of used sensors is now complete.

5.3.7 Configuring alarm groups

Configuration for associating events with certain alarm groups

By default, for the **Access Control** and **Detection Tools** alarm groups, no data is sent from *Agent Of Control*. These alarm groups, as well as **Hardware** and **Fire/Security System**, can be used for designating their respective alarm types.

To classify events of an object as belonging to a particular alarm group, create an object (if it does not exist already) in the device tree. For example, if you want for the signal from the **Motion detection tool** to be displayed in *Monitoring PSIM* in the **Detection Tools** alarm group, create a **Detector zone** object and configure it (select the **motion** type, specify the detection area and sensitivity, etc.; for more details, see [Axxon PSIM Software Package: Administrator's Guide](#)).

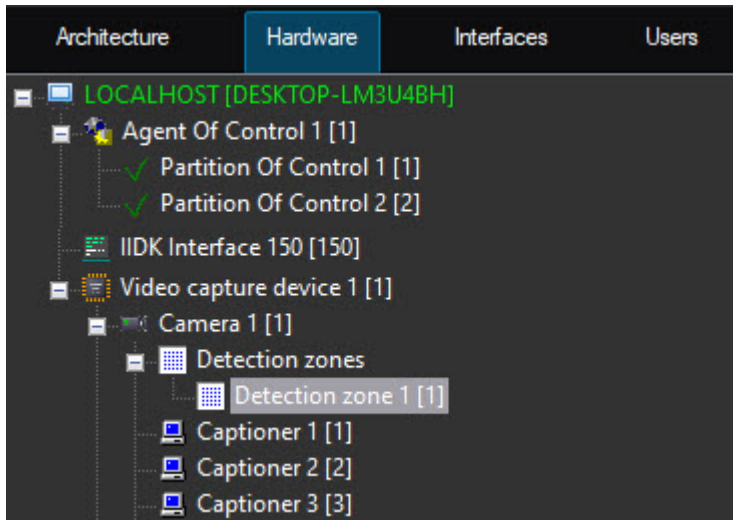

To associate the events with particular alarm groups, do the following:

1. Go to the configuration panel for the **Partition Of Control** object.

1 Partition Of Control 1 ID 386 Transmitting ...

Agent Of Control 1 TCP port (LPS) 8888 Monitoring ... 1

Video data ...

Number	Keep archive for (days)
1	60/0

Cameras ...

Total cameras: 1

Sensor ID	Sensor type
1	Vibration sensor (frames,captions)

Sensors

Add ...

Edit ...

Delete

Registration

No connection

Sensors: 1

Apply Undo

2. Click the **Monitoring...** button. The **Add/Edit events for Monitoring** window opens.

Add/Edit events for Monitoring

id	Type	Type (id)	Number	Name	Event	Event (id)	Group of alarms	Conf.	Video data	Message	Detail
----	------	-----------	--------	------	-------	------------	-----------------	-------	------------	---------	--------

Add ... Edit Delete

3. To add an event, click the **Add...** button. The event configuration window opens.

4. In the form that appears, from the **Type** drop-down list (1), select the type of device. This list contains the types of all objects created on the **Hardware** tab of the **System settings** window that have recorded events. Example: In the case of the **Motion detection tool**, select the **Detector zone** type.
5. From the **Number** drop-down list (2), select an ID number for the object of the selected type from which you want to get events. If you want to get events from all devices of this type, leave this field blank.
6. From the **Event** drop-down list (3), select the event type. The available event types depend on the selected object type. System type of the event in brackets is used in scripts and programs (see [Guide for creating scripts \(programming\)](#) and [The Script object. Programming using the JScript language](#)). For example, for the **Motion detection tool** triggering event, select **Alarm in the zone (MD_START)**.
7. From the **Group of alarms** drop-down list (4), select an alarm group and indicate in which alarm group you want for *Monitoring PSIM* to display alarms for this event.
8. It is possible to get confirmation of alarm acceptance from the *Server of Control*. To do this, from the **Confirmation** drop-down list (5), select the type of confirmation:
- No** – no confirmation is sent.
 - Simple** – *Agent of Control* sends confirmation when an alarm is confirmed by the operator.
 - Complex** – when accepting an alarm the operator must confirm it in the confirm box and after that the confirmation is sent.

Note


- The *Agent of Control* sends the **Confirmed: Monitoring PSIM event** message to *Axxon PSIM* core when there is the confirmation of alarm acceptance on the *Server of Control*. Scripts that use this event can be created in *Axxon PSIM* – see [Sample scripts for processing alarm confirmations](#).
- Confirmation sending can be disabled on the side of the *Server of Control* – see [Sending confirmations of alarm acceptance](#).

9. If it is necessary to attach video data to alarms, click the **Video data** button (6). As a result, the **Select configurations for video data transmitted** window will open.

Note

Configuration of the transmitted video data is described in [Setting up the configurations for transferred video data](#).

- a. Move the required configurations using the button (1) from the left list to the right. Remove a configuration from the right list to the left one by using the button (2).

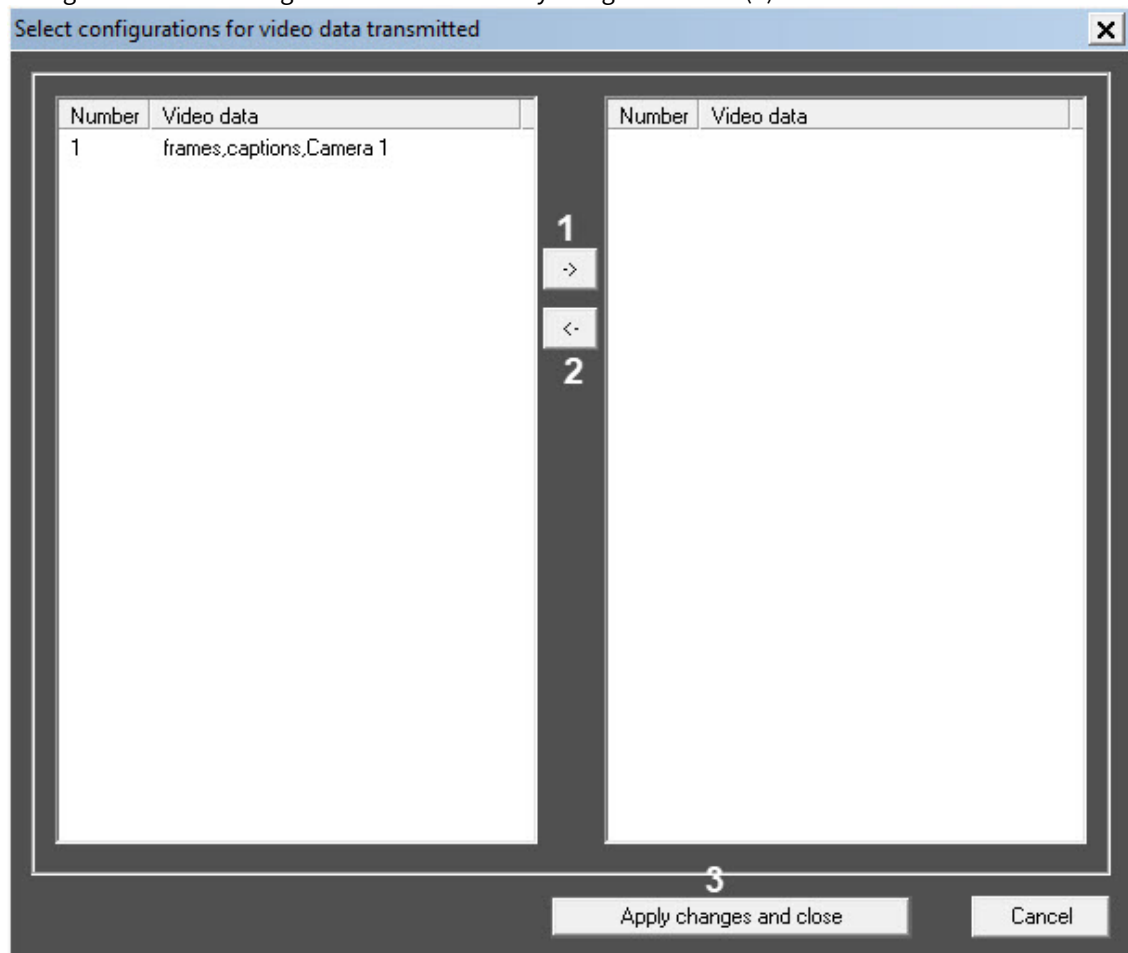**Attention!**

Multiple configurations cannot be used for the same camera.

- b. Click the **Apply changes and close** button (3). The selected configurations will be listed in the non-editable **Video data** field.
10. To add the possibility of attaching a snapshot not associated with the camera to an event, set the **Get snapshot from external device** checkbox (7). This way you can transmit, for example, a JPG snapshot received from an X-ray apparatus.

Attention!

To enable the **Get snapshot from external device** setting, the imageBase64<> substring with an image encoded in it must be present in the monitored event.

Example of an image received from an external device.



11. In the **Message** field (8), enter the text message, that will appear in the **Device** column of the **Reaction to alarm** dialog form (see [Monitoring PSIM Software Package: Operator's Guide](#)). If the object identifier is not specified, the following variables can be used in the **Message** field to detail the message:
 - a. <id> — identifier of the object from which the event came.
 - b. <name> — the object name.

⚠ Attention!

<id> and <name> are to be in lower case.
After substitution of variables values the message must not be longer than 60 characters. If the resulting message is longer, extra characters will be dropped.

📘 Example.

When the **Disarmed** event appears at the **Camera 1**, the **Camera 1 disarmed** message is sent.

The screenshot shows a dialog box with the following fields and values:

- Type: Camera
- Number: 1
- Event: Disarmed (DISARM)
- Group of alarms: Detections
- Confirmation: No
- Video data: Configuration [1]
- Get snapshot from external device:
- Message: Camera <id> disarmed
- Capture detailed data:

12. To search for additional information in messages from a device of this type (for the substring "param0<>"), set the **Capture detailed data** checkbox (9).
13. Click the **OK** button to save the changes (10).

This means that when integrating a new device into *Axxon PSIM*, if a developer wants to be able to send more detailed information to *Monitoring PSIM*, when generating an event from the device, the developer should add detail in the param0<> parameter. For example, if there is a Motherboard Control module that has the Alarm event, the following values could be included in param0<>: "processor cooler", "BIOS battery", etc. If you enter **Motherboard** in the **Message** field and select **Capture detailed data**, the following text may appear in the **Device** column of the **Reaction to alarm** dialog form: **Motherboard (CPU cooler)**.

Similarly, it is possible to monitor messages from other objects created in the *Axxon PSIM* device tree, on the **Hardware** tab.

Configuration for associating events with certain alarm groups is now complete.

Setting up the configurations for transferred video data

If the transmission of user alarms (see [Configuration for associating events with certain alarm groups](#) section) to the *Server of Control* is configured, then video data can be added to these alarms. The video data transmission configurations can be created in *Monitoring PSIM* software in order to be added to any events when configuring alarm groups.

Important!

If video data (snapshots or videos) is added to an alarm, then the script for stopping camera recording is to be created (see [Sample script for stopping camera recording](#) section).

Set up the configurations for transferred video data as follows:

1. Go to the settings panel of the **Partition Of Control** object.

1 Partition Of Control 1 ID 386 Transmitting ...

Agent Of Control 1 TCP port (LIPS) 8888 Monitoring ...

Video data ... 1

Number	Keep archive for (days)
1	60/0

Cameras ...

Total cameras: 1

Sensor ID	Sensor type
1	Vibration sensor (frames,captions)

Sensors: 1

Sensors: Add ... Edit ... Delete

Registration: No connection

Apply Undo

2. Click the **Video data...** button. The **Adding/Removing configurations for transferred video data** box appears.

Adding/Removing configurations for transferred video data

Number	Camera	Video data	Post-alarm time (s)	Pre-alarm time (s)	Number of frames	Interval (s)	Length (s)	Speed (Kbyte/s)	Export to avi	Captions	Show for (s)
--------	--------	------------	---------------------	--------------------	------------------	--------------	------------	-----------------	---------------	----------	--------------

Add ... Edit Delete

- To add a new video data transmission configuration click the **Add...** button. The configuration settings box appears.

- From the **Assignment to camera** drop-down list (1) select the **Camera** object that will be used for getting video data.
- Configure the data transmission parameters (2). The data transmission parameters are the same as those for video data transmitted along with sensor alarms (see [Configuring sensors](#) section, steps 7-15).
- Click the **OK** button (3). The created configuration is added to the list.
- Click the **Apply** button.

Setting up the configurations for transferred video data is complete.

Changing the description of short alarms and long alarm Object disarmed

To change the description of a long alarm **Object disarmed** in the **Monitoring** and **Monitoring reports** interface objects, it is necessary to specify the required description for the **CustomizedLongAlarmName** registry key on the *Server of Control* and *Central Server of Control* side (for details, see [Registry keys reference guide](#), for more information about working with the registry, see [Working with Windows OS registry](#)).

To change the description of short alarms that occur with the **OBJ_ARM** and **OBJ_DISARM** events, do the following:

- Run the *ddi.exe* utility on the *Agent of Control* side.

Note

For detailed information about working with this utility, see [Axxon PSIM Software Integration gGide \(HTTP API, IIDK, ActiveX\)](#).

- Open the *monitoring.ddi* file, which is located in the *<Axxon PSIM installation directory>\Languages\en*.
- Select the **VIDEOSRV_C** object (1).

4. Go to the **Events** tab (2).

DDI & DBI Editor - [C:\Program Files (x86)\Axxon PSIM\Languages\en\monitoring.ddi]

File

DDI DBI

Names **2** Events Reactions Icons States Transfer rules

Name	Description	Processing messages	Support audio	Disable network connection	Disable logging	Windows log
OBJ_DISARM	Attention! The service staff works!	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
OBJ_ARM	The object is armed	INFORMATION	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
*	3		<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Parameters for event "The object is armed":

Parameter	Name	Type	Element	Value
*				

Total objects: 13

5. In the **Description** column, specify the necessary text for the **OBJ_ARM** and **OBJ_DISARM** events (3).6. Save the changes to the file and restart the *Monitoring PSIM*.7. In the same way, select the **VIDEOSRV_S_DVC** object (1) on the *Server of Control* side.

DDI & DBI Editor - [C:\Program Files (x86)\Axxon PSIM\Languages\en\monitoring.ddi]

File

DDI DBI

Names **2** Events Reactions Icons States Transfer rules

Name	Description	Processing messages	Support audio	Disable network connection	Disable logging	Windows log
OBJECT_ARM	Object armed	INFORMATION	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
OBJECT_DI...	Object disarmed	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
MONITORIN...	Extra 1	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
MONITORIN...	Extra 2	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
*	3		<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Parameters for event "Object armed":

Parameter	Name	Type	Element	Value
*				

Total objects: 13

8. Go to the **Events** tab (2).9. In the **Description** column, specify the necessary text for the **OBJECT_ARM** and **OBJECT_DISARM** events (3).10. Save the changes to the file and restart the *Monitoring PSIM*.

Changing the description of short alarms and long alarm **Object disarmed** is complete.

Configuring alarms for monitoring the object state on the Agent of Control side

On this page:

- [General information about the alarms for monitoring of the object state on the Agent of Control side](#)
- [Configuring the alarms for monitoring the object state on the Agent of Control side](#)
- [Operating procedure](#)

General information about the alarms for monitoring of the object state on the Agent of Control side

To monitor the object state on the *Agent of Control* side, create an **AccessByCardEnable** string registry key and set **1** as its value (for details, see [Registry keys reference guide](#), for more information about working with the registry, see [Working with Windows OS registry](#)).

By default, the following alarms will become available in the **Detection Tools** alarm group:

Alarm group	Event name	Alarm type (default alarm description)	Alarm length
Detection Tools	-	Object disarmed	Long alarm
	OBJECT - DISARM	Attention! The service staff works!	Short alarm

	O B J - A R M	Armed object	Short alarm
--	---------------------------------	--------------	-------------

These alarms are designed for the special mode of *Monitoring PSIM* operation with *ACFA PSIM* (see [Configuring the special mode of Monitoring operation with ACFA PSIM](#)). However, these alarms can be used to monitor the state of the relay, for example, to generate a short and long alarm when the relay switches from the **Relay on** to the **Relay off** state, and another short alarm when the relay switches from the **Relay off** to the **Relay on** state.

Configuring the alarms for monitoring the object state on the Agent of Control side

You can change the description of alarms for the **OBJ_ARM** and **OBJ_DISARM** events, and the long alarm **Object disarmed** (for details, see [Changing the description of short alarms and long alarm Object disarmed](#)).

To receive the short alarms **Attention! The service staff works!** it is necessary to set up an alarm group as shown below.

To receive the short alarms **The object is armed**, it is necessary to set up an alarm group as shown below.

Note

It is necessary to enter the **<obj_disarmed>** and **<obj_armed>** messages in the lower case.

To monitor the object state on the *Agent of Control* side, do the following:

1. In the **System Settings** dialog box, go to the **Programming** tab (1).

2. Create the **Script** object (2) on the basis of the **Scripts** object in the objects tree.
3. If you are configuring the special mode of *Monitoring PSIM* operation with *ACFA PSIM*, it is necessary to copy the contents of a sample script from the page [Sample scripts for determining the current state of the zones of the Apollo object on the Agent of Control side.](#)

4. If you are configuring the monitoring of the relay state, it is necessary to copy the contents of a sample script from the page [Sample scripts for determining the current state of the relay on the Agent of Control side](#).
5. Click the **Apply** button (3).

Operating procedure

At startup, and then every 15 minutes, *Agent of Control* sends a **GET_OBJECT_STATE** event to the *Axxon PSIM* core. This event is processed in a script, which then generates an **OBJECT_STATE_INFO** event with the object status in the **state** field and the additional information in the **card** field. When the state of the relay changes, this script generates the **OBJ_ARM** or **OBJ_DISARM** event a long alarm **Object disarmed**.

Configuring alarms for monitoring the object state on the *Agent of Control* side is complete.

5.4 Connecting to uninterrupted power supplies

If your computer has a Smart-UPS uninterrupted power supply unit made by APS, messages from the UPS can be sent to *Server of Control*.

Configuration of a UPS is performed in the following order:

1. Install the StateUPS utility.
2. Configure the PowerChute plus utility.

5.4.1 Configuring StateUPS

StateUPS utility (exe-file and ini-file) is installed with *Agent of Control* and placed to the <*Axxon PSIM* software installation>/Vhost/UPS/.

Note

Files from the <*Axxon PSIM* software installation>/Vhost/UPS/Ext directory will look for the ini settings file in the same directory as the StateUPS utility.

Configure the file StateUPS.ini in this directory:

1. Address – address of the machine on which *Agent of Control* is running. The default value of this parameter is 127.0.0.1. If you install StateUPS on the same computer on which *Agent of Control* is installed, it is not necessary to change this parameter.
2. Port – TCP port to which StateUPS sends messages from the UPS. The value of this parameter must match the corresponding setting of *Agent of Control*, TCP port (UPS) (see the section [Configuring a port for incoming UPS messages](#)).


If the StateUPS utility is to be used on another computer, do the following:

1. Create HKLM\SOFTWARE\BitSoft\VHOST\VHostService section in the registry for 32-bit OS (HKLM\SOFTWARE\Wow6432Node\BitSoft\VHOST\VHostService for 64-bit) on this computer.
2. In this section, create the **FolderLog** parameter. In the **FolderLog** parameter specify the path where the UPS folder will be created containing INI-file. For example, if the folder is **C:\EVUPS**, then **FolderLog = C:\EVUPS**.
3. In the specified folder, for example, **C:\EVUPS**, create the UPS sub-folder and copy the StateUPS.ini into it.


5.4.2 Installing the software from the UPS vendor

After the StateUPS is configured, install the software from the UPS vendor. Before starting installation, make sure that the interface cable is connected to the UPS.


1. To start the installation process, start the executable file pc521.exe in the installation folder UPS\PowerChutePlus. A window opens to inform of the start of installation.

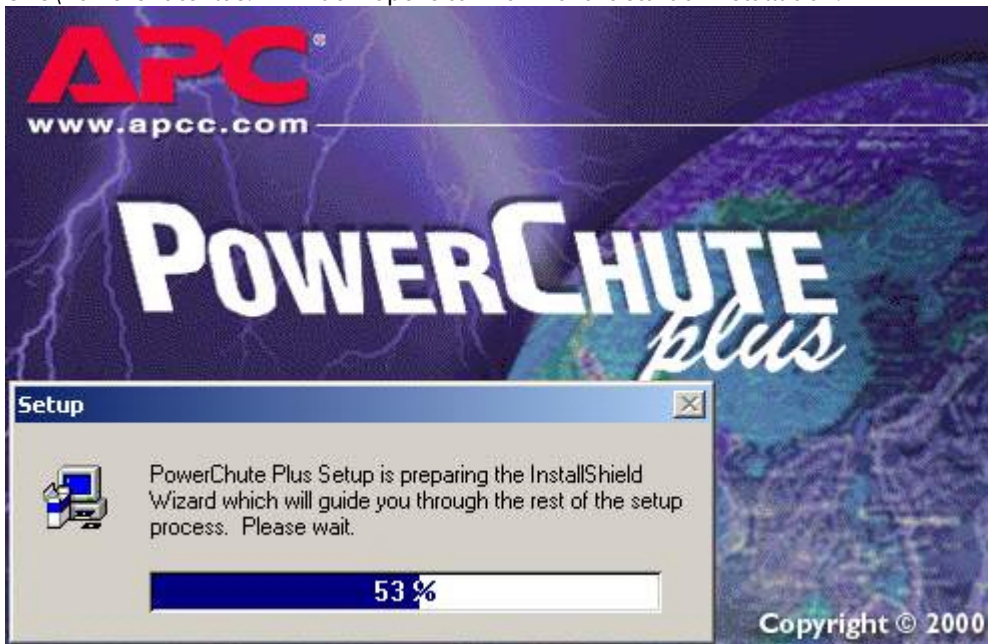


2. On the following wizard page, select the option **Continue with the installation now** and click the **Next** button.

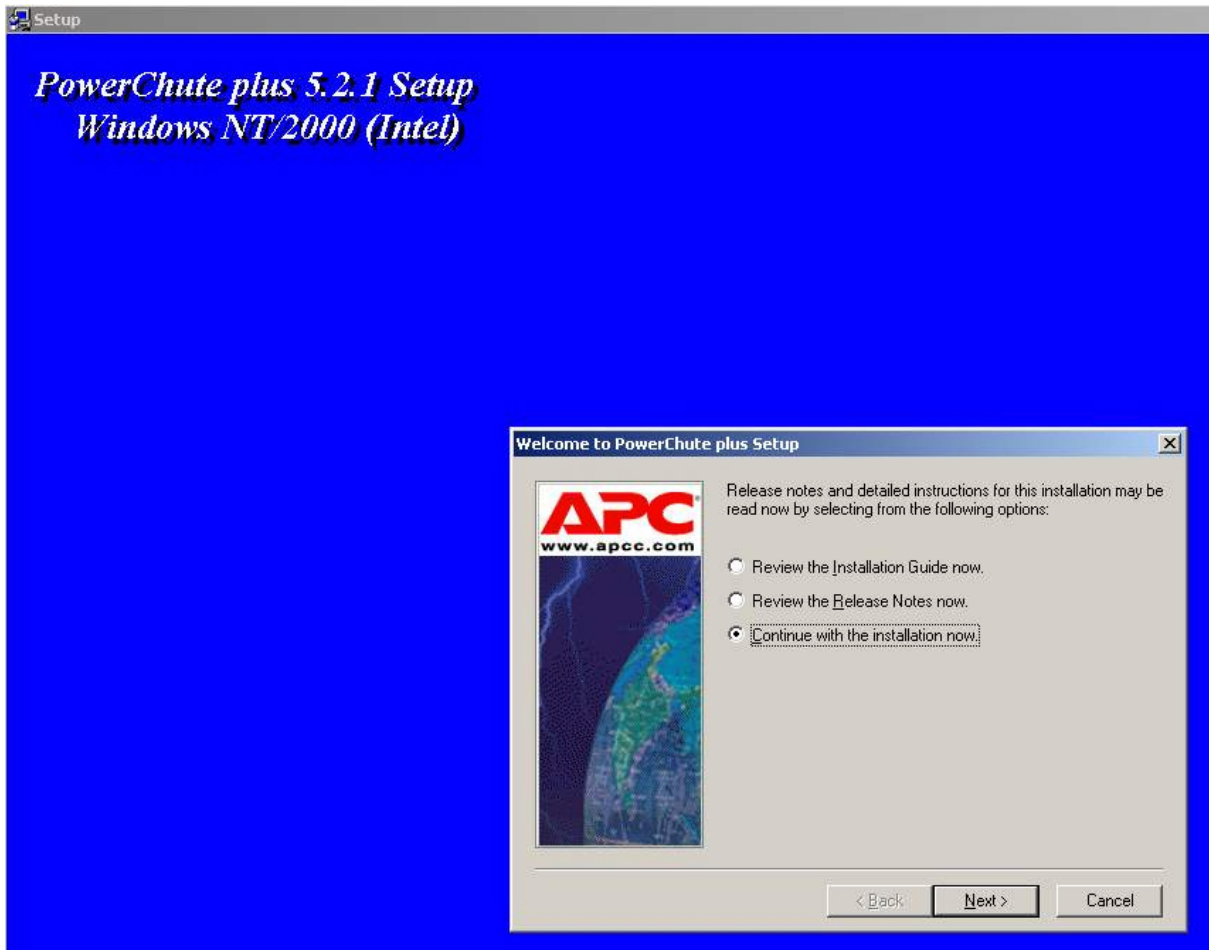


3. On the following wizard page, click the **Yes** button to accept the license agreement.

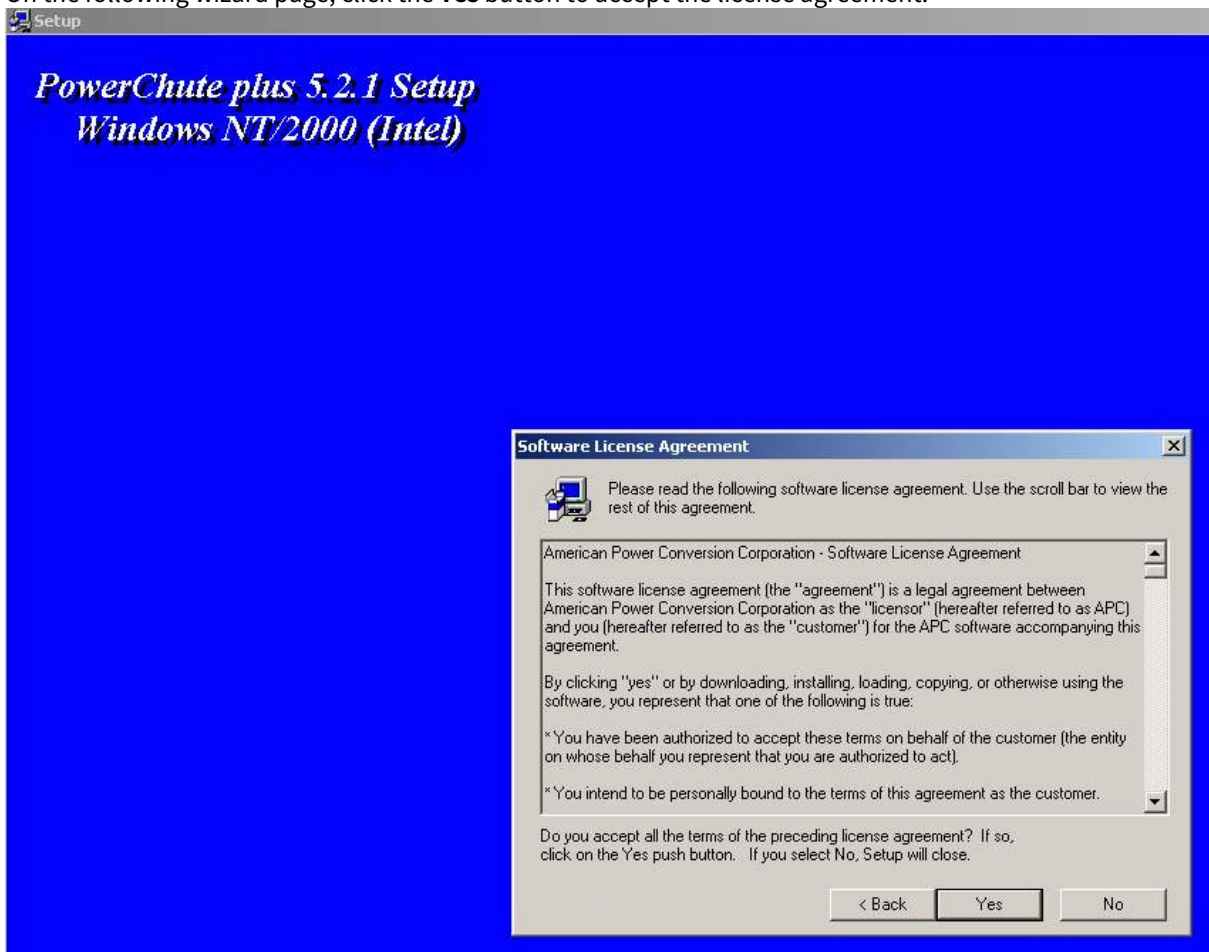


4. On the following wizard page, select the **Typical** installation type and indicate the path at which you want to install the software.

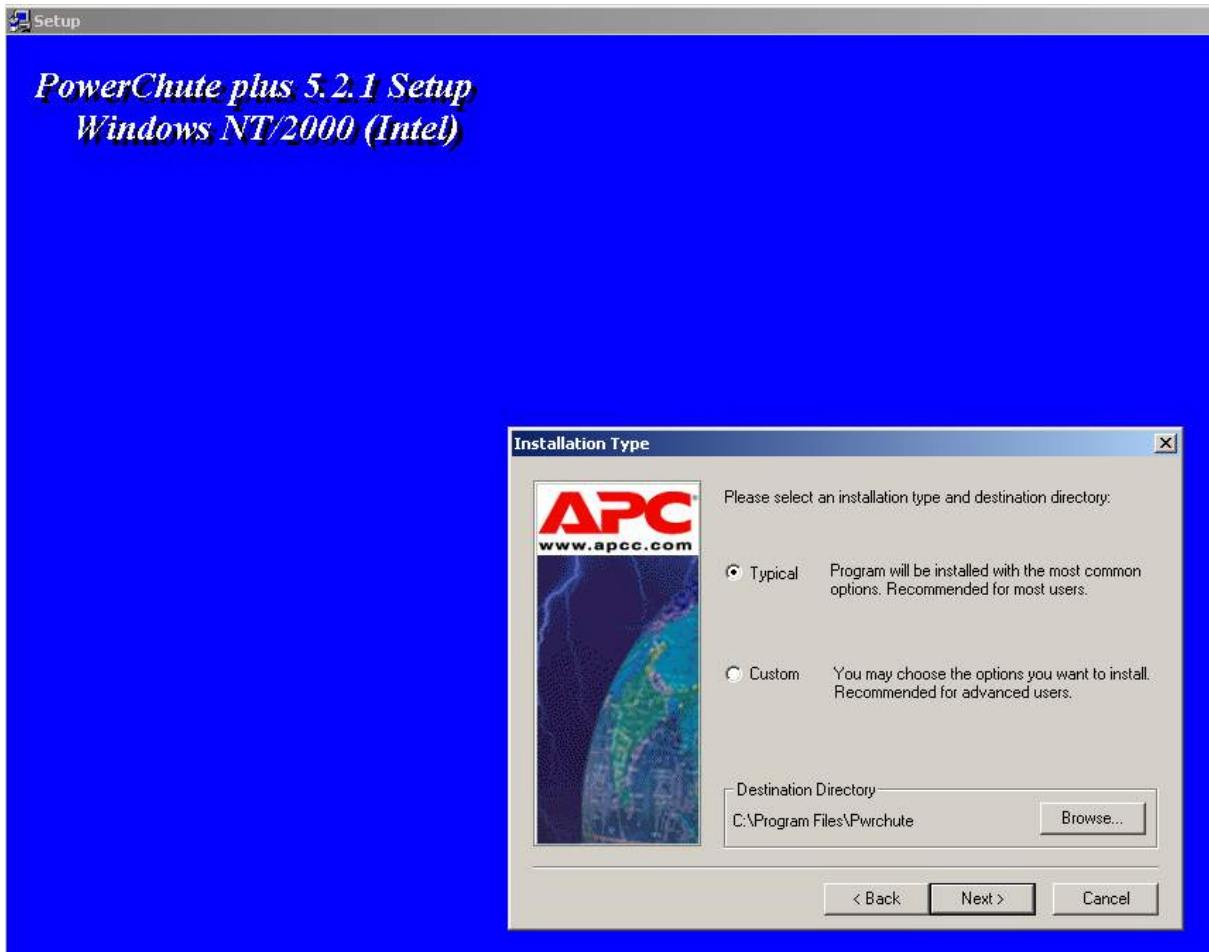


5. Copying begins of the necessary files.

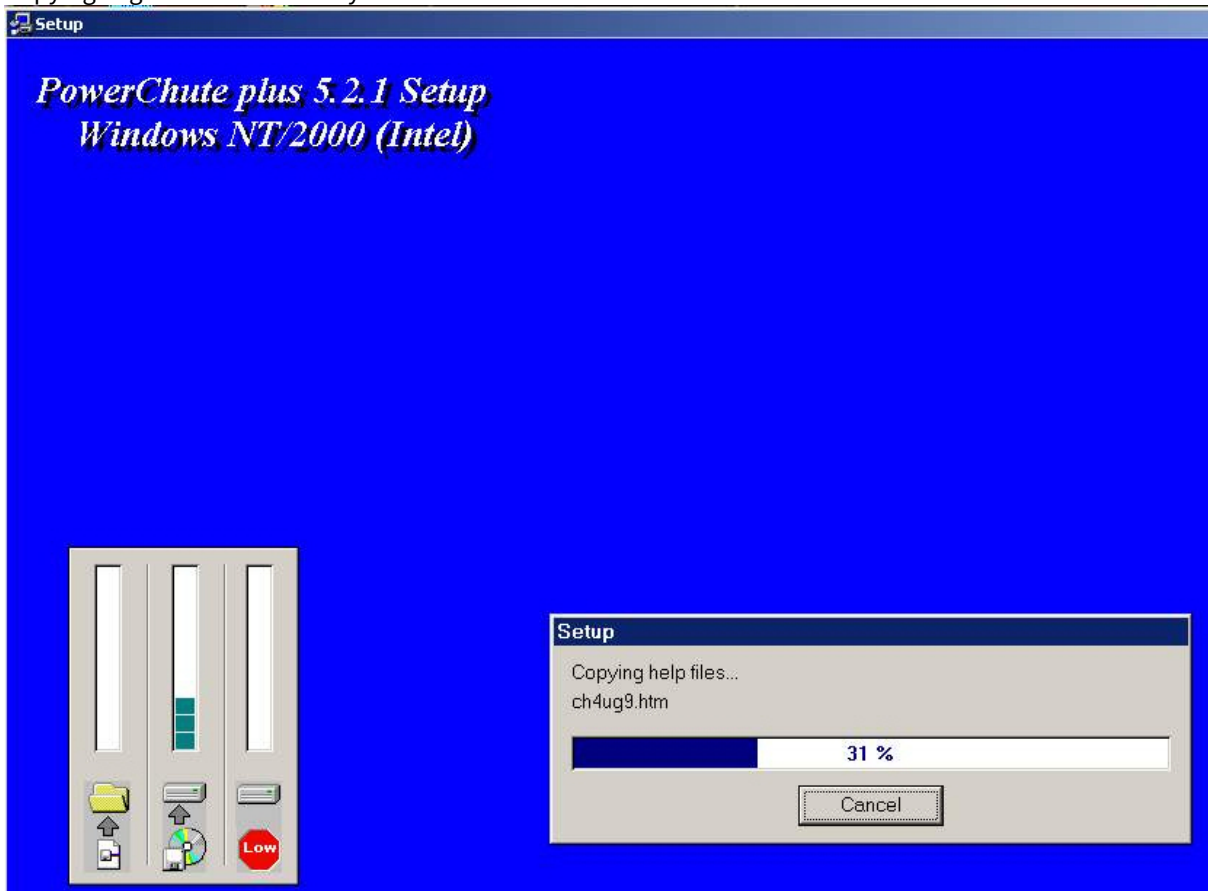


6. When copying is complete, a dialog box appears with a request to automatically determine the COM port on which the UPS is located. Click the **Yes** button.

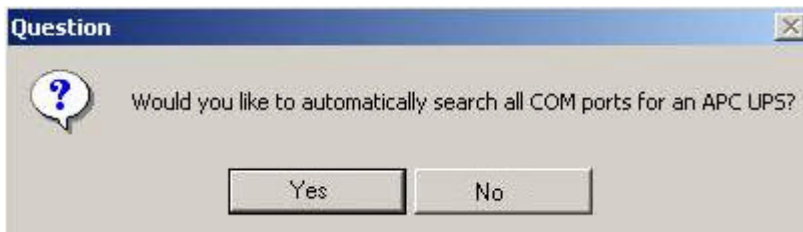


7. The search process begins.

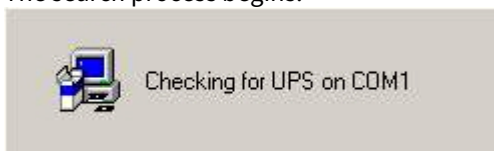


- When the search is complete, the program will show what type of UPS it found and on which COM port. Click the **Next** button.

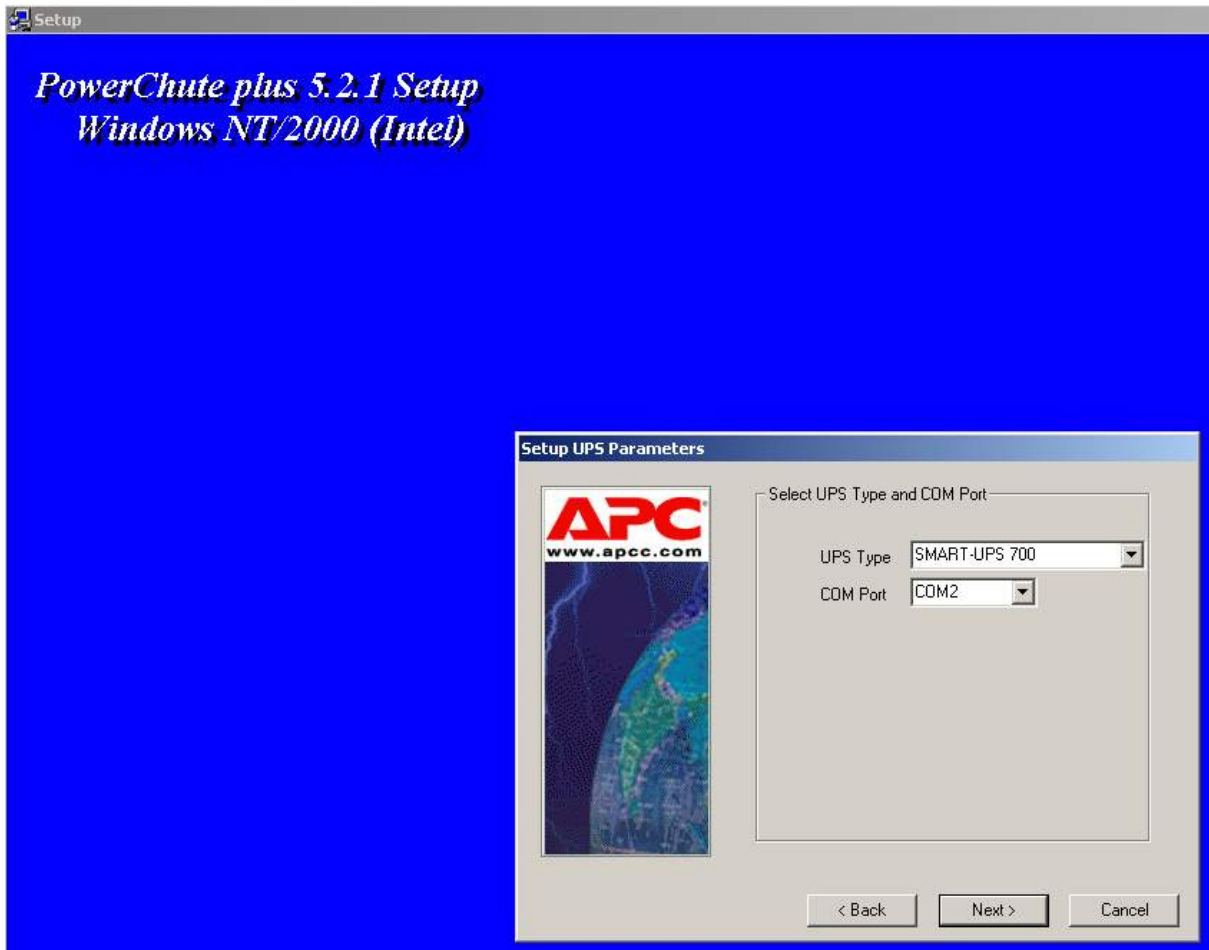

- On the next wizard page, clear the **Enable PowerChuteplus remote Monitoring PSIM** check box and click the **Next** button.

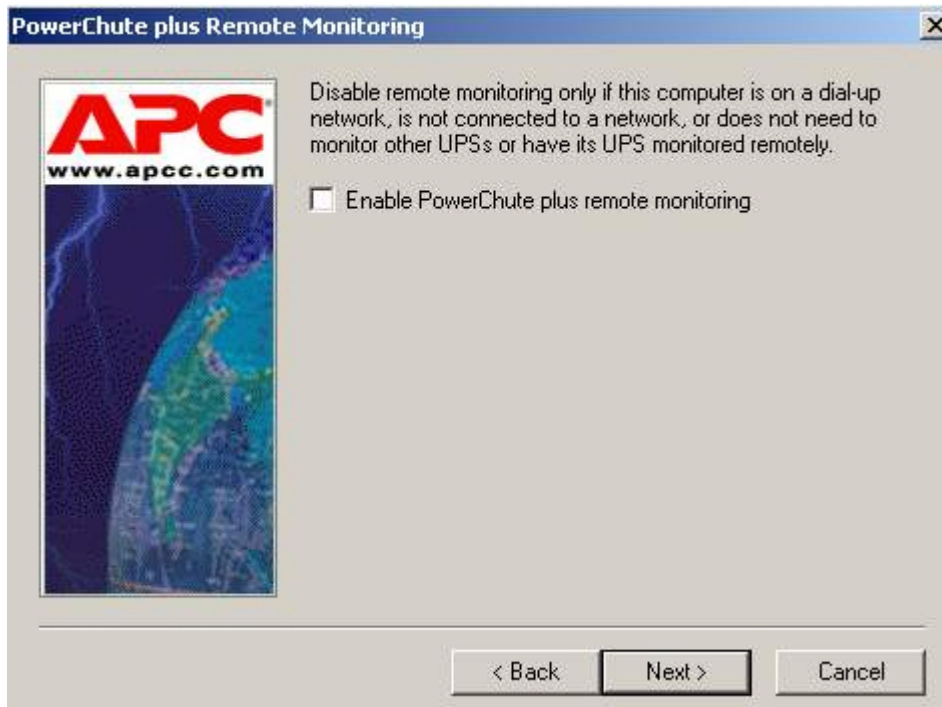

- The two following wizard pages complete the installation process.

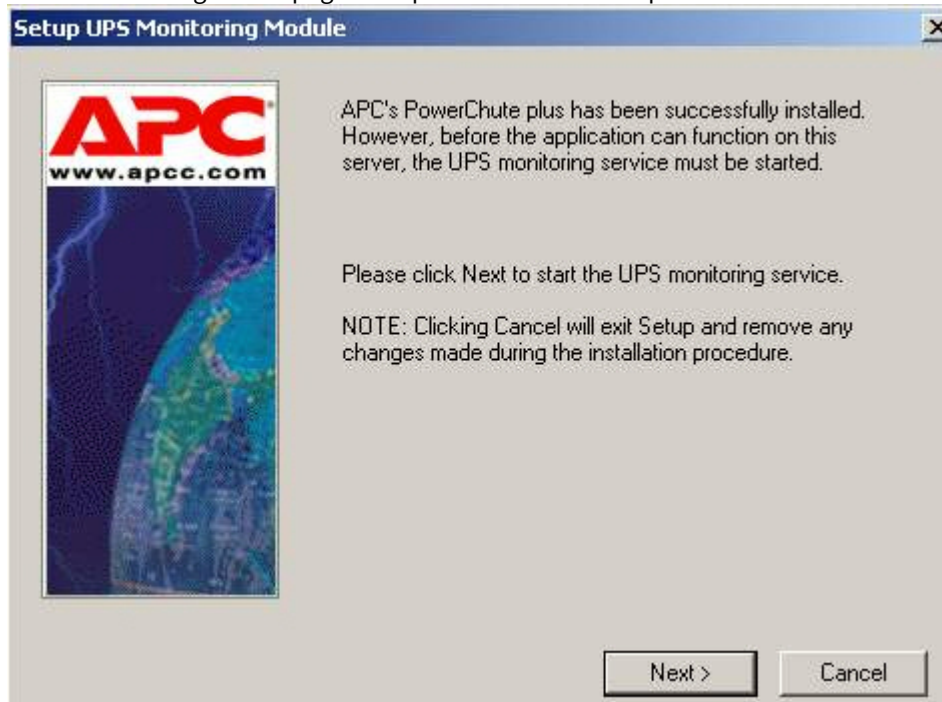

Dialog box to confirm installation completion.



Installation of the StateUPS utility is now complete.


5.4.3 Configuring the PowerChute plus utility

Note.


The PowerChute utility configuring process is given in this document as an example. Alternative software can have different settings. Alternative software must allow binding certain reactions with UPS events.

To set up the PowerChute plus utility:

1. Start the PowerChute plus configuration program, by selecting **Start -> Programs -> PowerChute plus -> PowerChute plus.**

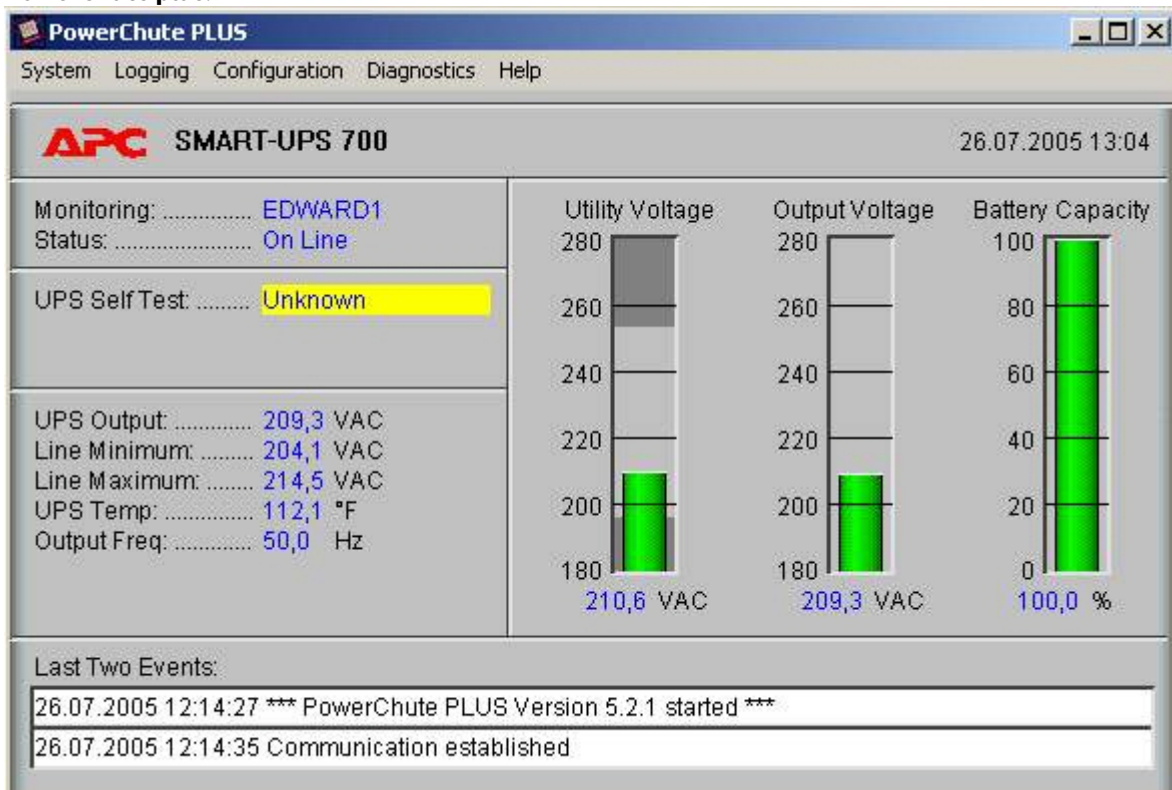

2. Select the menu item **Configuration -> Event Actions...** A dialog box appears, in the left part of which there is a list of events for which different reactions can be assigned (right part of the window). It is recommended to disable the **Notify Users** option for all events unless there is a need for it; otherwise, messages are sent to the entire domain on which the computer is located.

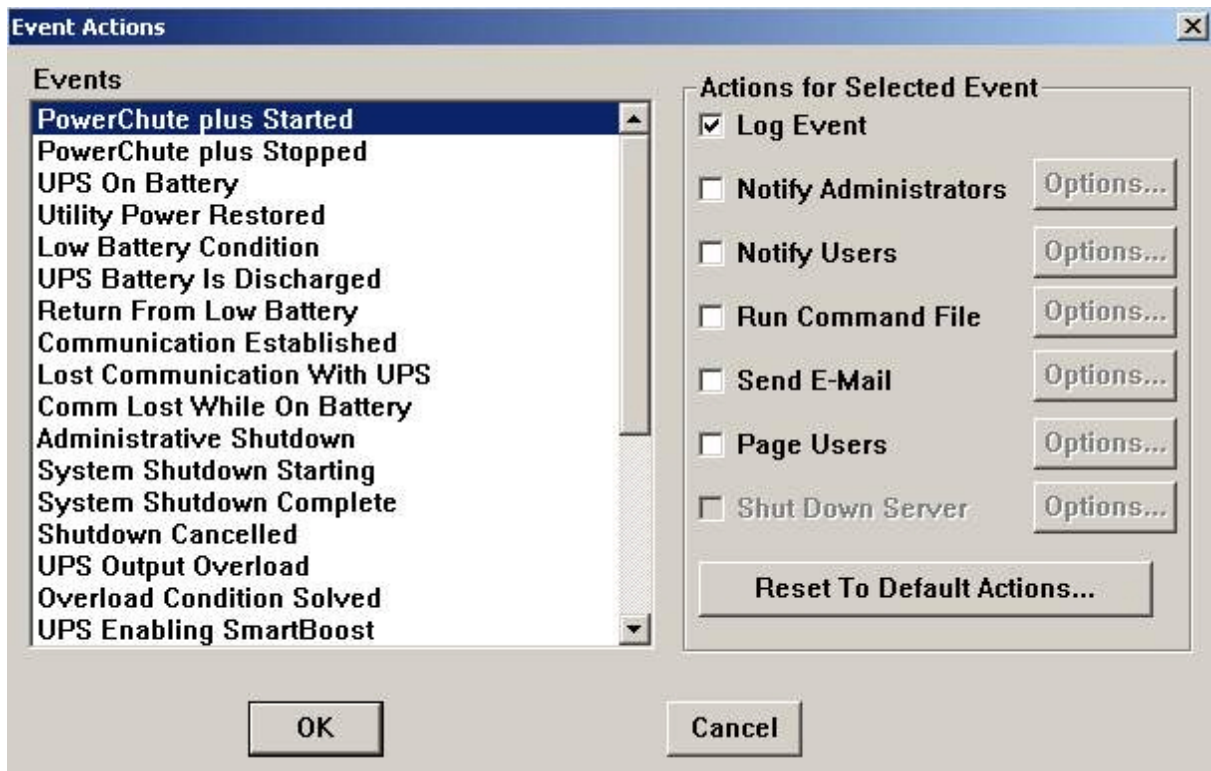

A more detailed list of events is given in the table.

ID Code	Event Name	Description
1000	PowerChute Started	PowerChute service started
1001	PowerChute Stopped	PowerChute service stopped
1002	Communication Established	Communication restored
1003	Utility Power Restored	Electricity restored
1004	UPS Self-Test Passed	Self-Test passed
1005	Administrative Shutdown	Administrative shutdown
1006	Shutdown Cancelled	Shutdown cancelled
1007	Returned From Low Battery	Battery charged
1009	UPS Battery Replaced	Battery replaced

1013	Overload Condition Solved	Overload is back to normal
1014	Runtime Calibration Started	Runtime Calibration Started
1015	Runtime Calibration Finished	Runtime Calibration Finished
1016	System Shutdown Starting	System is shutting down
1102	UPS Internal Temperature In Bounds	Internal temperature is in bounds
2000	UPS On Battery	Electricity turned off
2001	System Shutdown Complete	System performed shutdown
2002	UPS Enabling SmartBoost	Low-voltage mode
2003	Low Battery Condition	Battery is running low
2004	Runtime Calibration Aborted	Runtime Calibration Aborted
2007	UPS Enabling SmartTrim	High-voltage mode
3000	Lost Communication With UPS	Communication lost
3001	UPS Output Overload	Overload
3002	UPS Self-Test Failed	Self-Test failed
3003	UPS Battery Is Discharged	Battery discharged
3004	Comm Lost While On Battery	Comm Lost While On Battery
3016	Battery Needs Replacing	Must replace battery
3107	Maximum Internal Temperature Exceeded	High internal temperature

PowerChute plus can be configured so that any of the events listed previously can be sent to the *Server of control*.

Events marked in green are highly recommended for sending to *Server of control*.

The <Axxon PSIM installation>\Vhost\UPS\Ext\ folder also includes three executables that have been created for specific events:

- PowerOff.exe (electricity is off)

- PowerOn.exe (electricity is restored)
- BatDisch.exe (battery is discharged)


This minimal set can be used with different series of Back-UPS that do not support calling third-party subprograms with the command line.

5.4.4 Example of configuration of event distribution


Let us consider the following situation: electricity has turned off and the UPS began to work in battery mode (ID Code = 2000), and after a time electrical supply was restored (ID Code = 1003).

In this case to configure events notifying do the following:

1. In the list of events, select the event **UPS On Battery** and, for this event, select the **Run Command File** check box.


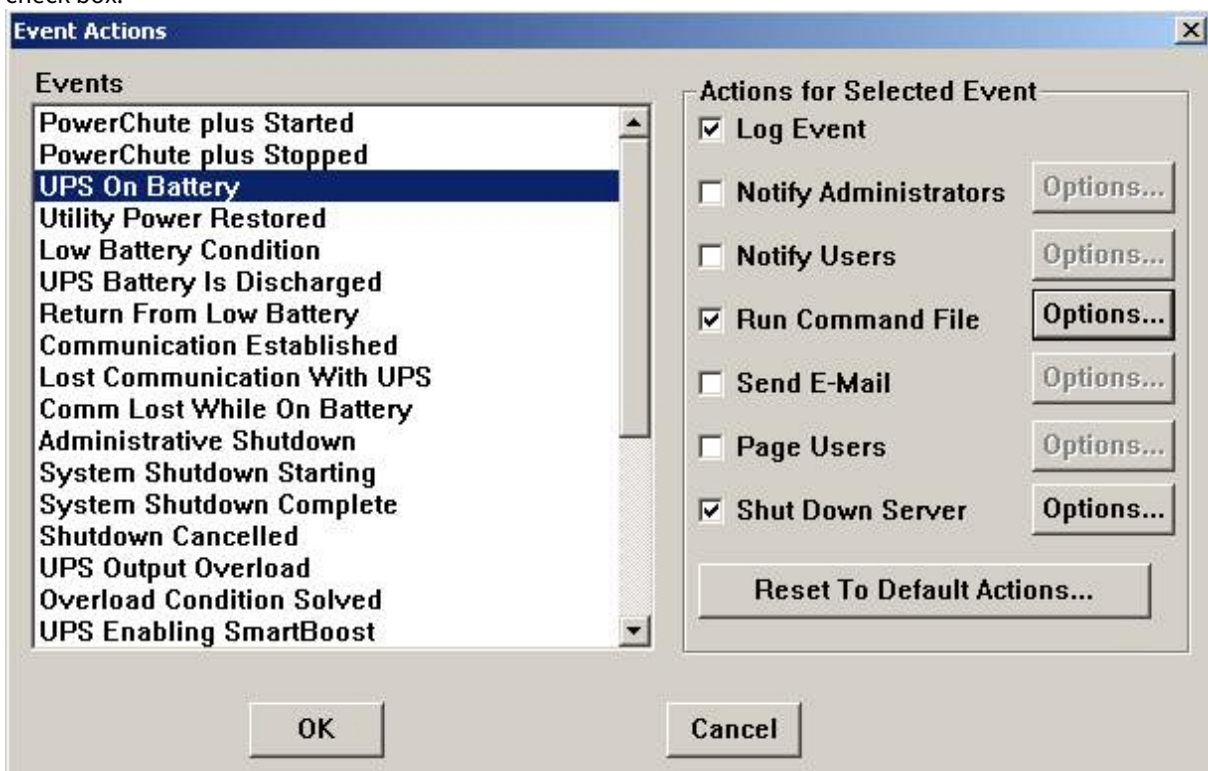


2. To the right of **Run Command File**, click the **Options...** button.
3. In the dialog box that opens, indicate the full path to the StateUPS utility that you want to be started when the event occurs.

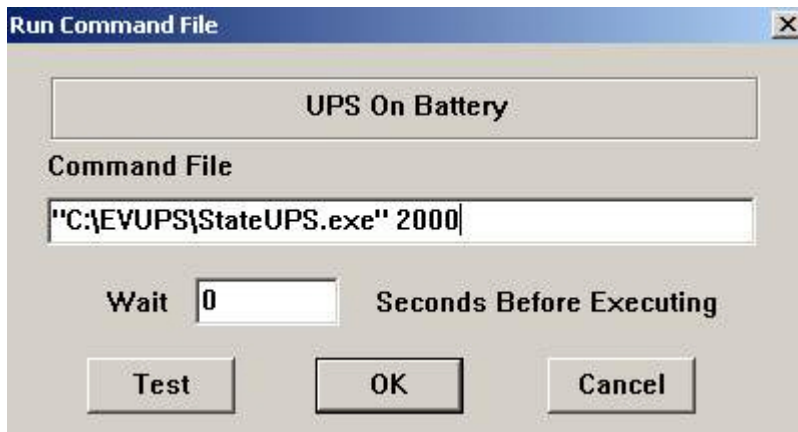

This path should be surrounded by double quotation marks (one at the beginning of the path and one at the end). Leave a space and then indicate the ID code; for the **UPS On Battery** event, the ID code is 2000.

4. Similar actions for the **Utility Power Restored** event are shown in the following figures.

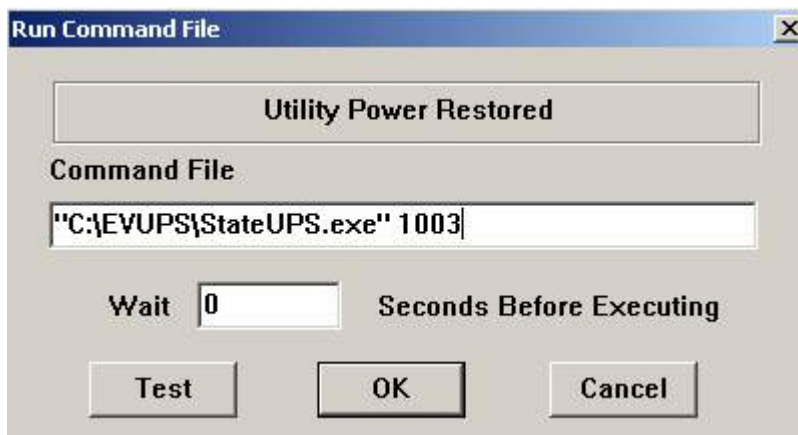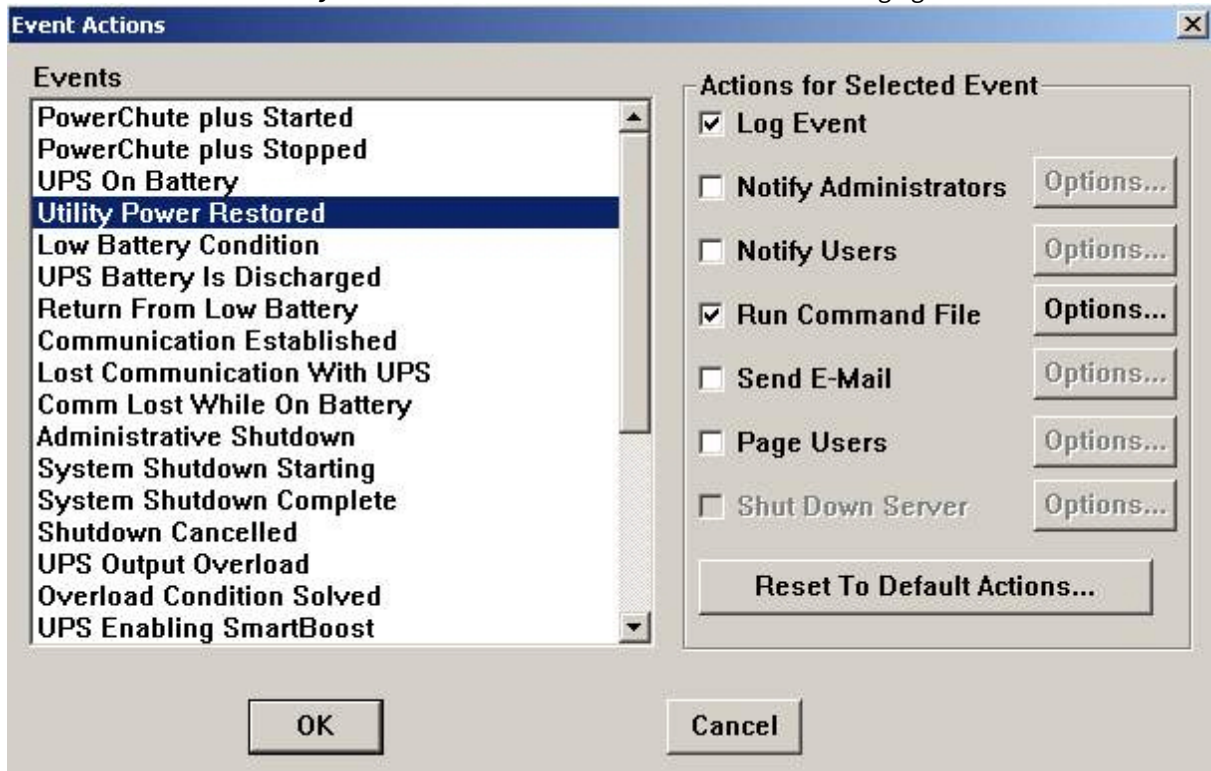

You should also remember that after utility power is restored, the UPS does not always generate the **Utility Power Restored** event; sometimes, it generates the **UPS Enabling SmartBoost** or **UPS Enabling SmartTrim** events. In order to not "miss" the moment at which utility power is restored, it is advisable to also handle the **UPS Enabling SmartBoost** and **UPS Enabling SmartTrim** events.

Each time the StateUPS utility is called, a log file is created in the <Axxon PSIM installation>\Vhost\UPS folder with a name of the following format:

```
upslog_<state><date><time>.log
```

5.5 Working with Agent of control without Windows administration rights

To allow the user not added to the Administrators group in the Windows operating system to work correctly with *Agent of Control*, make sure the following conditions are fulfilled:

1. The user must have full access to the *Agent of Control* registry section:
HKEY_LOCAL_MACHINE\Software\BitSoft for 32-bit system
(HKEY_LOCAL_MACHINE\Software\Wow6432Node\BitSoft for 64-bit).
2. The user must have full rights for the folder <DISK>:\Backup, where <DISK> is the logical disc where *Axxon PSIM* software is installed.

6 Configuring Server of Control

To configure *Server of Control*, go to the **System settings** window. Use of this window is described in [Axxon PSIM Software Package: Administrator's Guide](#).


6.1 Creating necessary Server Of Control objects

Note


Agent Of Control, like *Server Of Control*, can operate in a distributed configuration, while *Agents Of Control*, *Servers Of Control* and *Central Servers Of Control* can see where each of them is installed and can be configured.

To create necessary *Server Of Control* objects, do the following:

1. Go to **Hardware** tab in the **System settings** dialog box.
2. Create an **IIDK interface** object on the basis of the **Computer** object. Set the **IIDK Interface** object identifier (1).

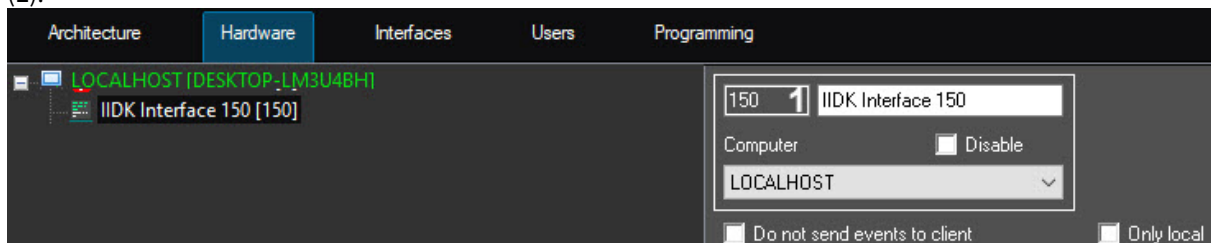


3. Create a **Server Of Control** object on the basis of a **Computer** object. On the settings panel of this object, in the **IIDK interface** field (2), enter the identifier of the previously created **IIDK Interface** object.

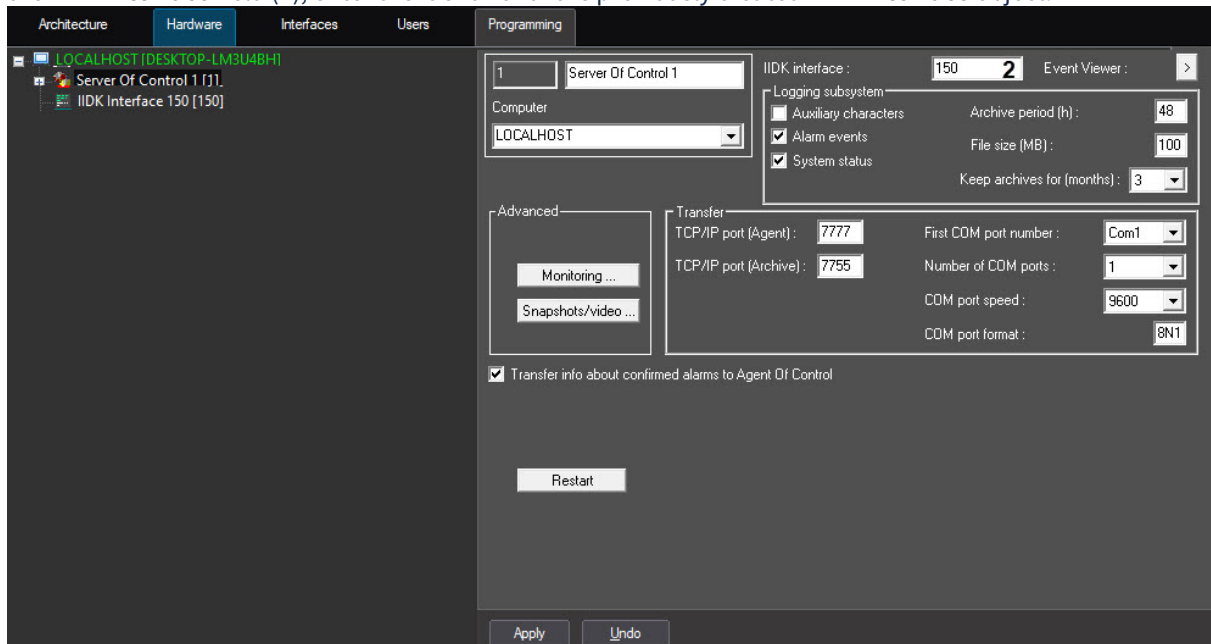

4. Create the required number of **Partition Of Control** child objects on the basis of the **Server Of Control** object. When you create these objects, specify the same ID (3) as in the **ID** field on the settings panel of the

corresponding **Partition Of Control** object created on the basis of the **Agent Of Control** object.

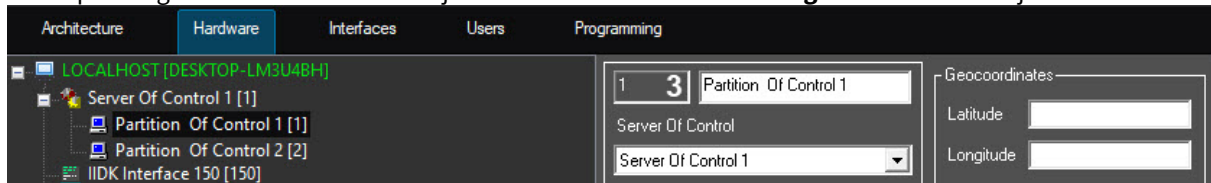

Note

It is not necessary to manually create the **Partition Of Control** objects on the basis of the **Server Of Control** object. They will be created automatically upon successful configuration of the communication between the *Agent Of Control* and the *Server Of Control* with the name and identifier specified on the *Agent Of Control* side (see [Configuring communication between Agent Of Control and Server Of Control](#)).

The required objects are now created.

6.2 Configuring a connection

A *Server Of Control* can simultaneously operate with objects over both the TCP/IP and RS232 protocols.

To configure a connection between *Server Of Control* and *Agent Of Control/Archive*, do the following:

1. Go to the settings panel of the **Server Of Control** object.

2. In the **TCP/IP port (Agent)** field, enter the port number for TCP/IP communication with remote objects (1).
3. In the **TCP/IP port (Archive)** field, enter the port number for TCP/IP communication with the *Search in archive* module (2).

Note

The default value of the **TCP/IP port (Archive)** is **7755**. After you change the port number, it is necessary to also change the **IPPort** registry key value to the new port number (for details, see [Registry keys reference guide](#). For more information about working with the registry, see [Working with Windows OS registry](#)).

4. For the RS232 protocol, configure the following parameters: **First COM port number**, **Number of COM ports**, **COM port speed**, and **COM port format** (3).
5. Click the **Apply** button.

Configuring a connection is complete.

6.3 Configuring logging subsystem

The logging subsystem allows configuring the detail level at which *Server of Control* activities are logged.

The main log file is located in the <Axxon PSIM software installation folder>\VHost folder, in the file vsrvYYMMDD.log, where YY is the year, MM the month, and DD the day.

To configure the logging subsystem:

1. Go to the configuration panel for the **Server Of Control** object.

The screenshot shows the configuration panel for the 'Server Of Control' object. The 'Logging subsystem' section is highlighted with numbered callouts 1 through 6. Callout 1 points to the 'Auxiliary characters' checkbox, 2 to the 'Alarm events' checkbox, and 3 to the 'System status' checkbox. Callout 4 points to the 'Archive period (h)' field (value 48), 5 to the 'File size (MB)' field (value 100), and 6 to the 'Keep archives for (months)' field (value 3). The 'Transfer' section shows 'TCP/IP port (Agent): 7777', 'TCP/IP port (Archive): 7755', 'First COM port number: Com1', 'Number of COM ports: 1', 'COM port speed: 9600', and 'COM port format: 8N1'. The 'Advanced' section has 'Monitoring...' and 'Snapshots/video...' buttons. The 'Transfer info about confirmed alarms to Agent Of Control' checkbox is checked. A 'Restart' button is at the bottom. The 'IIDK interface' is 150 and 'Event Viewer' is open.

2. To log auxiliary characters at the transport level, select the **Auxiliary characters** checkbox (1).
3. To log alarms (activation of a vibration sensor, temperature sensor, or Door-Forced-Open (DFO) sensor), select the **Alarm events** checkbox (2).
4. To log events related to system status, select the **System status** checkbox (3).
5. In the **Archive period (h)** field, enter the frequency, in hours, at which the log file is to be archived (4). Archives are saved in the DATA subfolder, with the following name format: `namelog_yymmddhhmmss.gz`, where
 - a. `namelog` is the name of the log file being archived;
 - b. `yy` is the year of archive creation;
 - c. `mm` is the month of archive creation;
 - d. `dd` is the day of archive creation;
 - e. `hh` is the hour of archive creation;
 - f. `mm` is the minute of archive creation;
 - g. `ss` is the second of archive creation.
6. In the **File size (MB)** field, enter the file size threshold, in megabytes, upon which the log file is archived (5). This setting overrides the value in the **Archive period (h)** field.


7. In the **Keep archives for (months)** drop-down list, select the length of time, in months, for which you want to store archived log files. This value must be between 1 and 24 **(6)**. Archives that are older than the specified number of months are deleted.

To save settings, click the **Apply** button.

6.3.1 Specifying storage time for event log

To specify the term of keeping the event log in the database do the following:

1. Go to the **Programming** tab of the **System settings** dialog box **(1)**.

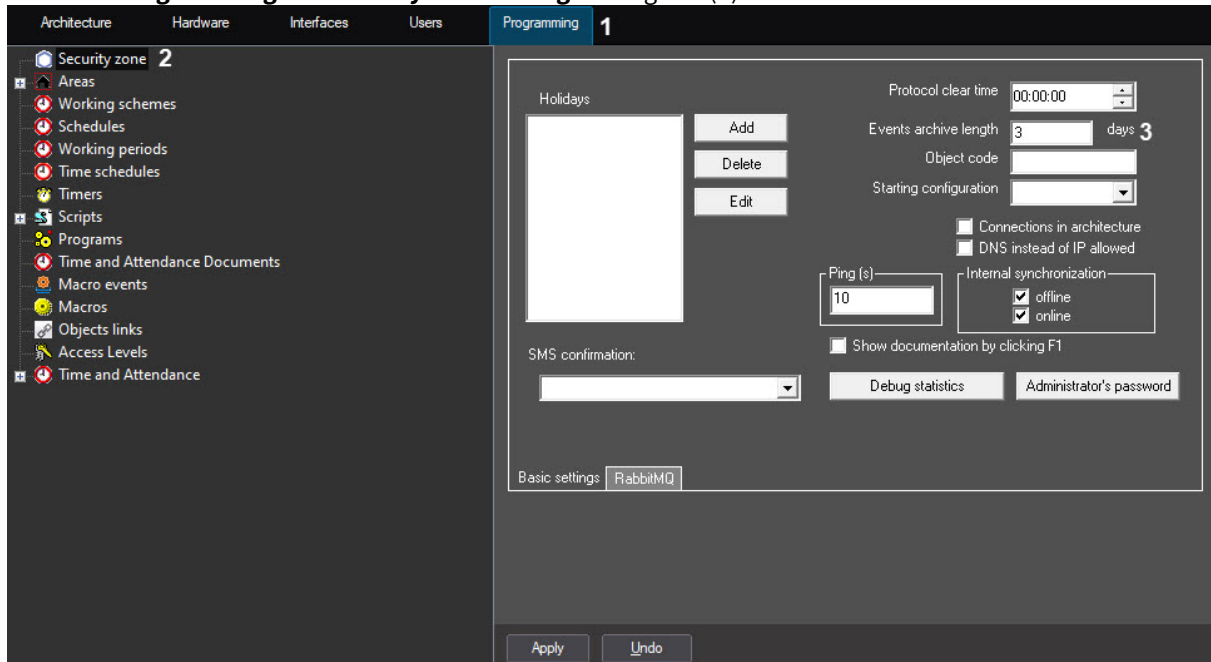

2. Go to the **Security zone** object setting panel **(2)**.
3. Specify the term of keeping the event log in the **Event archive length...days** parameter **(3)**.
4. Press **Apply**.

Specifying the term of keeping the event log is completed.

6.3.2 The Event Viewer utility

The disadvantage of viewing information via the *Event Viewer* is clearing the screen on each *Axxon PSIM* restart. It is impossible to see what was on before the system restart. The additional *Event Viewer* utility is required in such cases. This utility operates the database directly and allows to view information from the whole length of time used to keep the event log in the database.

To start the *Event Viewer* utility, click the **Event Viewer** button **(1)** on the **Server Of Control** settings panel.

1 Server Of Control 1 IIDK interface : 150 Event Viewer : > 1

Computer
LOCALHOST

Logging subsystem

Auxiliary characters Archive period (h) : 48

Alarm events File size (MB) : 100

System status Keep archives for (months) : 3

Advanced

Monitoring ...

Snapshots/video ...

Transfer

TCP/IP port (Agent) : 7777 First COM port number : Com1

TCP/IP port (Archive) : 7755 Number of COM ports : 1

COM port speed : 9600

COM port format : 8N1

Transfer info about confirmed alarms to Agent Of Control

Restart

Apply Undo

The *Event Viewer* utility allows to sort and filter data.

Event Viewer

Source	Event	Additional information	Date	Time
47 John Reed str.	Communication channel : failure		3/9/2023 1:43:01 PM	3/9/2023 1:43:02 PM
10 Green spruce dr.	Communication channel : failure		3/9/2023 1:43:01 PM	3/9/2023 1:43:02 PM
18 Alexanderplatz	Communication channel : failure		3/9/2023 1:43:01 PM	3/9/2023 1:43:02 PM
10 Green spruce dr.	Communication channel : failure		3/9/2023 11:53:53 AM	3/9/2023 11:53:53 AM
18 Alexanderplatz	Communication channel : failure		3/9/2023 11:53:53 AM	3/9/2023 11:53:53 AM
47 John Reed str.	Communication channel : failure		3/9/2023 11:53:53 AM	3/9/2023 11:53:53 AM
47 John Reed str.	Communication channel : failure		3/9/2023 11:36:03 AM	3/9/2023 11:36:03 AM

Records: 7

View records beginning with : 3/9/2023 Object : All objects

6.4 Configuring reaction to snapshots and videos

To configure the visualization of video frames and video fragments that are received with alarms (see [Viewing video data on alarms](#)), it is necessary to do the following:

Note.

This setting doesn't affect the acquisition of video data by the **Search in archive** interface object, except for the **AVI-files player** parameter (see [Request for video clips from objects](#)).

1. Go to the settings panel of the **Server Of Control** object and click the **Snapshot/video...** button (1).

The screenshot shows the configuration interface for the 'Server Of Control' object. The 'Advanced' section is expanded, and the 'Snapshot/video...' button is highlighted with a red box and the number 1. The 'Transfer' section is also visible, showing various port and COM settings.

Server Of Control 1

Computer: LOCALHOST

IIDK interface: 150 Event Viewer: >

Logging subsystem:

- Auxiliary characters
- Alarm events
- System status

Archive period (h): 48

File size (MB): 100

Keep archives for (months): 3

Advanced:

- Monitoring ...
- Snapshot/video ... 1**

Transfer:

TCP/IP port (Agent): 7777 First COM port number: Com1

TCP/IP port (Archive): 7755 Number of COM ports: 1

COM port speed: 9600


COM port format: 8N1

Transfer info about confirmed alarms to Agent Of Control

Restart


Apply Undo

A window will open where you can configure reactions to receiving snapshots and video.

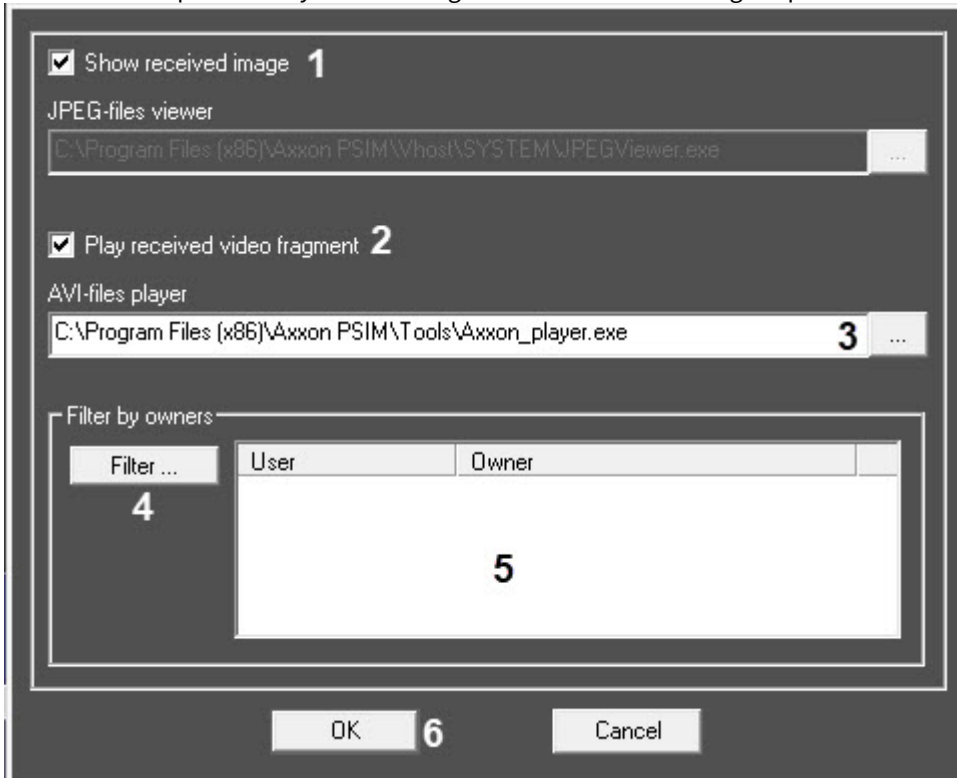

2. If you want to open the received image:
 - a. Set the **Show received image** checkbox (1).
3. If you want to playback the received video fragment:
 - a. Set the **Playback received video fragment** checkbox (2).
 - b. In the **AVI-files player** field, specify the path to the program used to playback the AVI files (3).
4. If you want certain users to have access only to snapshots and video fragments received from the objects belonging to specific owners, set a filter by owners:
 - a. Click the **Filter** button (4).

- b. The **Filter by owners** window will open. The list of available user-owner pairs is on the left (1), the list of the selected users and owners is on the right (2).

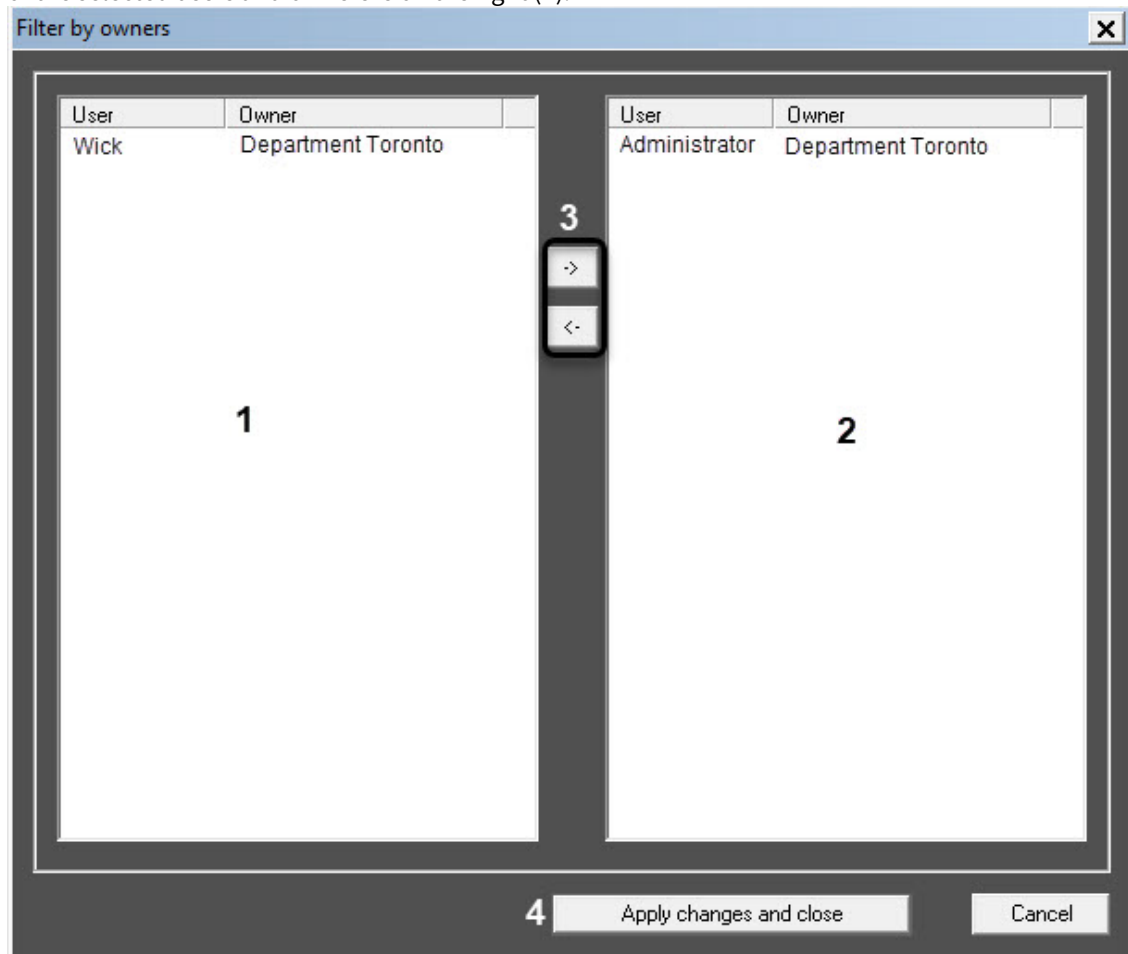

Note.

The list of owners is set on the **Control panel** (see [Regulatory and reference information](#)). Users and their rights are configured in the **Users** tab of the **System settings** dialog box (see *Axxon PSIM. Administrator's Guide*. The latest version of this document is available in [AxxonSoft documentation repository](#)).

- c. Move the pairs between the lists using the -> and <- buttons (3).
- d. When the list of users and owners is formed, click the **Apply changes and close** button (4).
5. Selected pairs of users and owners will be displayed in the table (5).
6. Click the **OK** button (6) to return to the settings panel of the **Server Of Control** object.
7. Click the **Apply** button.

Configuring reactions to receiving snapshots and video fragments is now complete.

6.5 List of Additional workplaces

For the *Additional workplaces* software operation, it is necessary to configure the list of additional workplaces on the *Server of Control*, and specify the computer name and the client code for each of them.

The client code is bound to the computer hardware. You can find it out as follows:

1. On the computer with installed *Monitoring PSIM*, open the **Search in archive** interface in the Additional workplace configuration.

ID	Camera	Date and time	Text
550016	Camera 1 [1]	3/7/2023 2:44:39 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:44:35 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:44:20 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:44:16 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:44:04 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:44:02 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:43:11 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:43:07 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:42:36 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:42:32 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:42:25 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:42:13 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:41:14 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:40:59 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:40:35 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:40:32 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:40:24 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:38:16 PM	Record on disk stopped
550016	Camera 1 [1]	3/7/2023 2:38:14 PM	Harddisk rec
550016	Camera 1 [1]	3/7/2023 2:38:07 PM	Record on disk stopped

2. Click the **Settings** button in the bottom left corner.
3. The client code is specified in the opened **Settings** box.

Settings

Connection to videosrv

IP address: 127.0.0.1

Port: 7755

Client code: BD6CA

Task archive size (days): 100

Maximum length of loaded video clip, sec: 120

Save Cancel


The list of Additional workplaces that can be connected to the *Server of Control* is configured as follows:

1. Go to the settings panel of the **Server Of Control** object and click the **Monitoring** button (1).


The screenshot shows the configuration window for a 'Server Of Control' object. At the top left, the object name is 'Server Of Control 1' and the computer is set to 'LOCALHOST'. The 'IIDK interface' is set to '150' and the 'Event Viewer' is expanded. Under 'Logging subsystem', 'Alarm events' and 'System status' are checked. The 'Archive period (h)' is 48, 'File size (MB)' is 100, and 'Keep archives for (months)' is 3. In the 'Transfer' section, 'TCP/IP port (Agent)' is 7777, 'TCP/IP port (Archive)' is 7755, 'First COM port number' is Com1, 'Number of COM ports' is 1, 'COM port speed' is 9600, and 'COM port format' is 8N1. A checkbox 'Transfer info about confirmed alarms to Agent Of Control' is checked. A 'Restart' button is located at the bottom left. At the bottom of the window are 'Apply' and 'Undo' buttons. A red box with the number '1' highlights the 'Monitoring ...' button in the 'Advanced' section.

As a result, the window for configuring the list of Additional workplaces will open.

- To add an Additional workplace to the list, click the **Add** button (2).

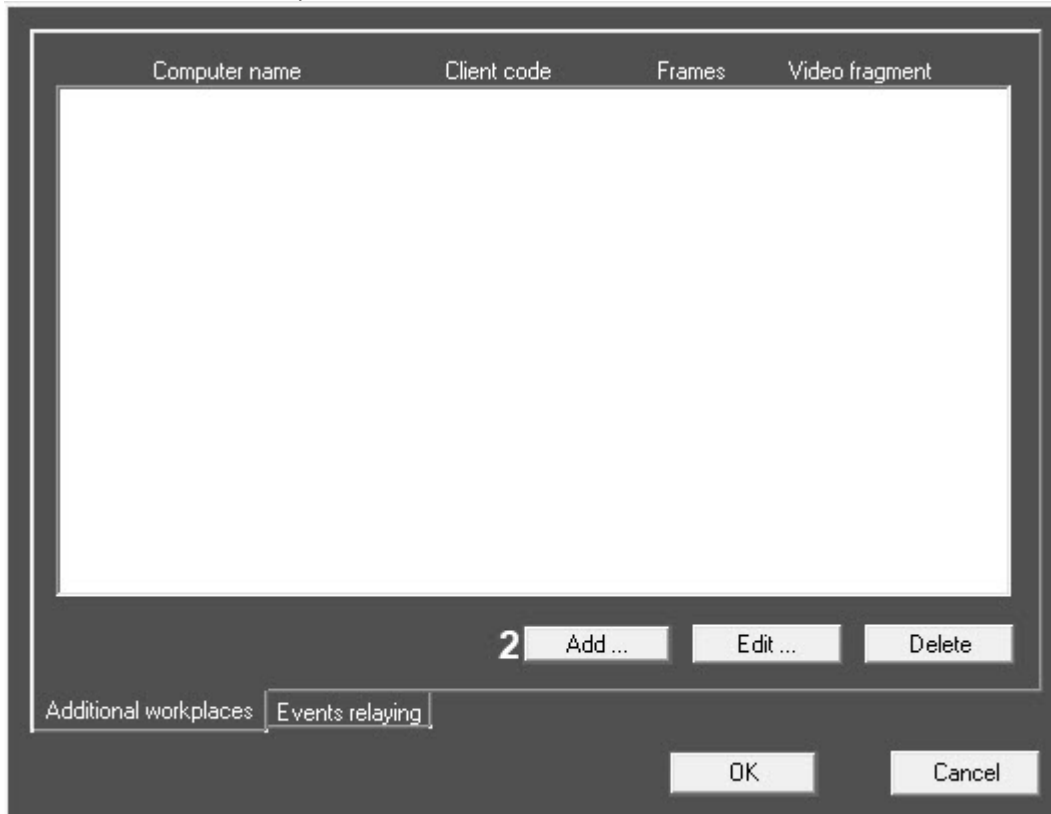

- In the opened window specify the computer name on which the Additional workplace is installed (1).

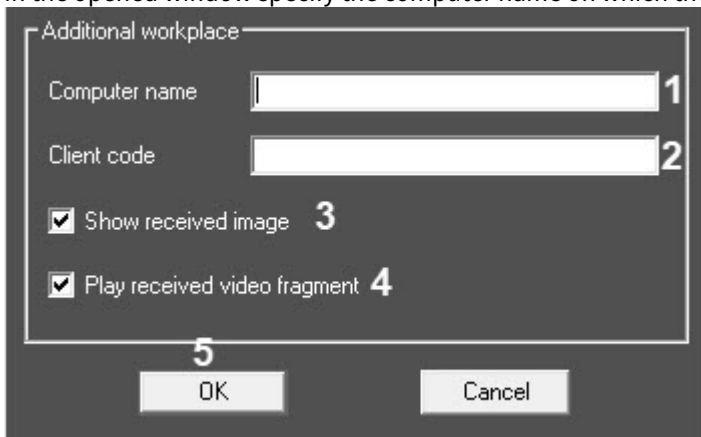

- In the **Client code** field (2), enter the client code.
To configure the visualization of video frames and video fragments that are received with alarms (see [Viewing video data on alarms](#)), it is necessary to do the following:

Note

This setting doesn't affect the acquisition of video data by the **Search in archive** interface object (see [Request for video clips from objects](#)).

- Set the **Show received image** checkbox (3) if you want to open the received video frames. The **Filter by owners** setting is taken into account (see [Configuring reaction to snapshots and videos](#)).

6. Set the **Play received video fragment** checkbox (4) if you want to playback the received video fragments. The **Filter by owners** setting is taken into account (see [Configuring reaction to snapshots and videos](#)).
7. Click the **OK** button (5) to save changes and return to the window for configuring the list of Additional workplaces.
8. Repeat steps 3-8 for all Additional workplaces that will be connected to this *Server of Control*.

 **Note**

To edit the specified settings, select the Additional workplace in the list and click the **Edit** button.
To delete the Additional workplace in the list, select it in the list and click the **Delete** button.

9. Click the **OK** button to save changes and return to the settings panel of the **Server Of Control** object.
10. Click the **Apply** button.

The list of Additional workplaces is now configured.

6.6 Sending confirmations of alarm acceptance

In general, the *Agent Of Control* is considered not to have the same core as the *Server Of Control*.

It is possible to configure sending messages to *Agent Of Control* when the operator confirms an alarm on the *Server Of Control*. The *Agent Of Control* then sends these messages to *Axxon PSIM* core. Two types of confirmation are available: simple and complex. The confirmation type is selected when configuring alarm transmission to the *Server Of Control* (see [Configuration for associating events with certain alarm groups](#)).

When the confirmation is sent, the *Server Of Control* waits for the confirmation from the *Agent Of Control* that the message has been sent to *Axxon PSIM* core. If this message is not received, then confirmation packets are sent every 5 minutes.

 **Note**

See also [Sample scripts for processing alarm confirmations](#).

Disable sending confirmations of alarm acceptance as follows:

1. Go to the settings panel of the **Server Of Control** object.

2. Clear the **Transfer info about confirmed alarms to Agent Of Control** checkbox (1).

The screenshot shows the configuration interface for the Server of Control. At the top, there are fields for 'IIDK interface' (set to 150) and 'Event Viewer'. Below this is the 'Logging subsystem' section with checkboxes for 'Auxiliary characters', 'Alarm events', and 'System status', along with fields for 'Archive period (h)' (48), 'File size (MB)' (100), and 'Keep archives for (months)' (3). The 'Transfer' section includes fields for 'TCP/IP port (Agent)' (7777), 'TCP/IP port (Archive)' (7755), 'First COM port number' (Com1), 'Number of COM ports' (1), 'COM port speed' (9600), and 'COM port format' (8N1). The checkbox 'Transfer info about confirmed alarms to Agent Of Control' is checked and marked with a red circle and the number 1. At the bottom left, the 'Apply' button is marked with a red circle and the number 2. Other buttons include 'Monitoring ...', 'Snapshots/video ...', 'Restart', and 'Undo'.

3. Click the **Apply** button (2).

The **Transfer info about confirmed alarms to Agent Of Control** function is now disabled.

6.7 Working with Server of Control without Windows administration rights

To allow the user not added to the Administrators group in the Windows operating system to work correctly with *Server of Control*, make sure the following conditions are fulfilled:

1. The user must be given full access to the registry key:
 - For a 32-bit system: HKEY_LOCAL_MACHINE\Software\BitSoft
 - For a 64-bit system: HKEY_LOCAL_MACHINE\Software\Wow6432Node\BitSoft
2. The user must be granted full rights to the export directory (see [Specifying the export directory](#)).

6.8 Configuring sound notification at Server of Control

6.8.1 Configuring sound notification at Servers Of Control in a general way

Monitoring PSIM allows configuring audio signal that accompanies alarm messages received from *Agents Of Control*. For this, do the following:

Note


This function is not supported for the *Additional Workstation* in non-distributed configuration.

1. Create a **Display** object in the **Interfaces** tab.
2. Create an **Audio player** object on the basis of the **Display** object.
3. Run the *System configuration* utility (ddi.exe).

Note

Detailed information on using this utility is given in the *Axxon PSIM software. Administrator's Guide*. The most relevant version of this document is available in [AxxonSoft documentation repository](#).

4. Open the monitoring.ddi file.
5. Select the VIDEOSRV_S_DVC (**Partition Of Control**) object (1).
6. Go to the **Events** tab (2).

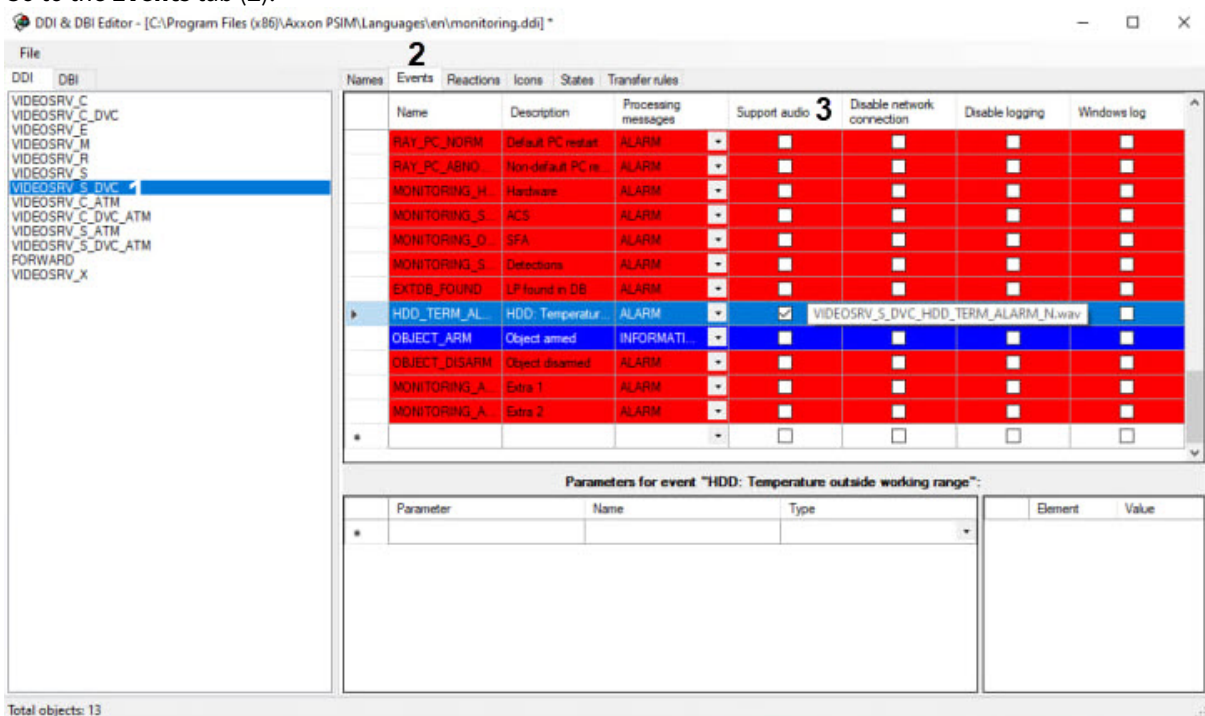

7. In the **Support audio** column, set the checkboxes next to all events that have to be accompanied by an audio signal (3).
A tooltip shows the required name of the WAV file.
N is an ID of the VIDEOSRV_S_DVC object.
8. Create corresponding files and place them into the <Axxon PSIM installation>\Wav folder.

Configuration of sound notification at *Server Of Control* is completed.

6.8.2 Configuring sound notification at Server Of Control for various alarm groups

There are four alarm groups in *Monitoring PSIM*. Several different events can be assigned to them at the *Agent Of Control*. These groups are: **Hardware, ACS, SFA, Detections** (see [Configuration for associating events with certain alarm groups](#)).

In order to configure sound notification for alarm groups, do the following:

Note

This function is not supported for the *Additional Workstation* in non-distributed configuration.

1. Create and configure the **Display** and **Audio player** objects in the **Interfaces** tab of the **System settings** dialog box.
2. Run the *System configuration* utility (ddi.exe).

Note

Detailed information on using this utility is given in the *Axxon PSIM software. Administrator's Guide*. The most relevant version of this document is available in [AxxonSoft documentation repository](#).

3. Open the monitoring.ddi file, select the VIDEOSRV_S_DVC (**Partition Of Control**) object (1).
4. Go to the **Events** tab (2).

DDI & DBI Editor - [C:\Program Files (x86)\Axxon PSIM\Languages\en\monitoring.ddi] *


Name	Description	Processing messages	Support audio	Disable network connection	Disable logging	Windows log
RAY_PC_NORM	Default PC restart	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
RAY_PC_ABNORM	Non-default PC r...	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
MONITORING_HR	Hardware	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
MONITORING_SKD	ACS	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
MONITORING_OPS	SFA	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
MONITORING_SENS	Detections	ALARM	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
EXTDB_FOUND	LP found in DB	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
HDD_TERM_ALARM	HDD. Temperatu...	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
OBJECT_ARM	Object armed	INFORMATI...	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
OBJECT_DISARM	Object disarmed	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
MONITORING_ADD1	Extra 1	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
MONITORING_ADD2	Extra 2	ALARM	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Parameters for event "Detections":

Parameter	Name	Type	Element	Value
*				

Total objects: 13

5. Make sure that the **Support audio** is not (3) set for the **Detections** event.
6. Close the *System configuration* utility.
7. Create and configure the **Program** object in the **Programming** tab of the **System settings** dialog box.

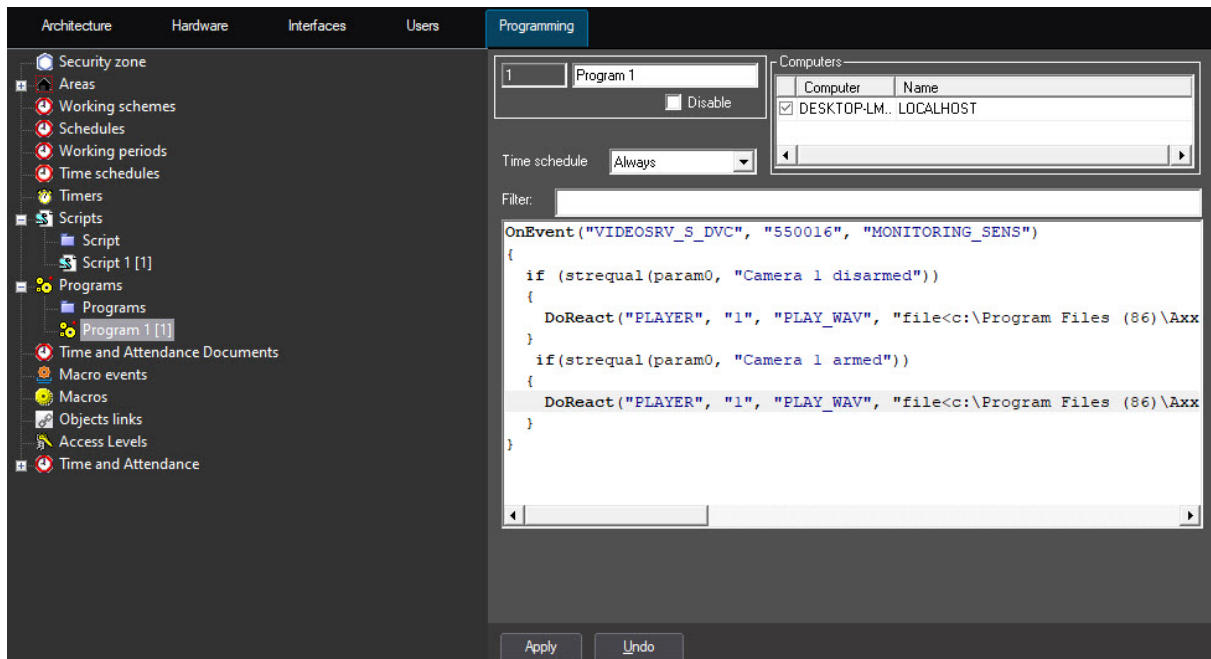

Example of a program for alarm groups is shown in the figure:

id	Type	Type (id)	Number	Name	Event	Event (id)	Group of alarms	Conf.	Video data	Message	Detail
1	Camera	CAM	1	Camera 1	Disarmed	DISARM	Detections	No	No	<name> disarmed	
2	Camera	CAM	1	Camera 1	Armed	ARM	Detections	No	No	<name> armed	

```

OnEvent("VIDEOSRV_S_DVC","550016","Monitoring_SENS")
{
  if (strequal(param0, "Camera 1 disarmed"))
  {
    DoReact("PLAYER","1","PLAY_WAV","file<c:\Program Files (x86)\Axxon
PSIM\Wav\cam_disarm.wav>");
  }
  if (strequal(param0, "Camera 1 armed"))
  {
    DoReact("PLAYER","1","PLAY_WAV","file<c:\Program Files (x86)\Axxon
PSIM\Wav\cam_arm.wav>");
  }
}


```


8. Create the corresponding files and place them into the <Axxon PSIM installation>\Wav folder.

Configuration of sound notification at *Server Of Control* for various alarm groups is completed.

6.9 Configuring the Server of Control from another server in a distributed configuration

To configure the *Server of Control* from another server in a distributed configuration, do the following:

1. Go to the settings panel of the **Server Of Control** object.
2. Click the  button (1).

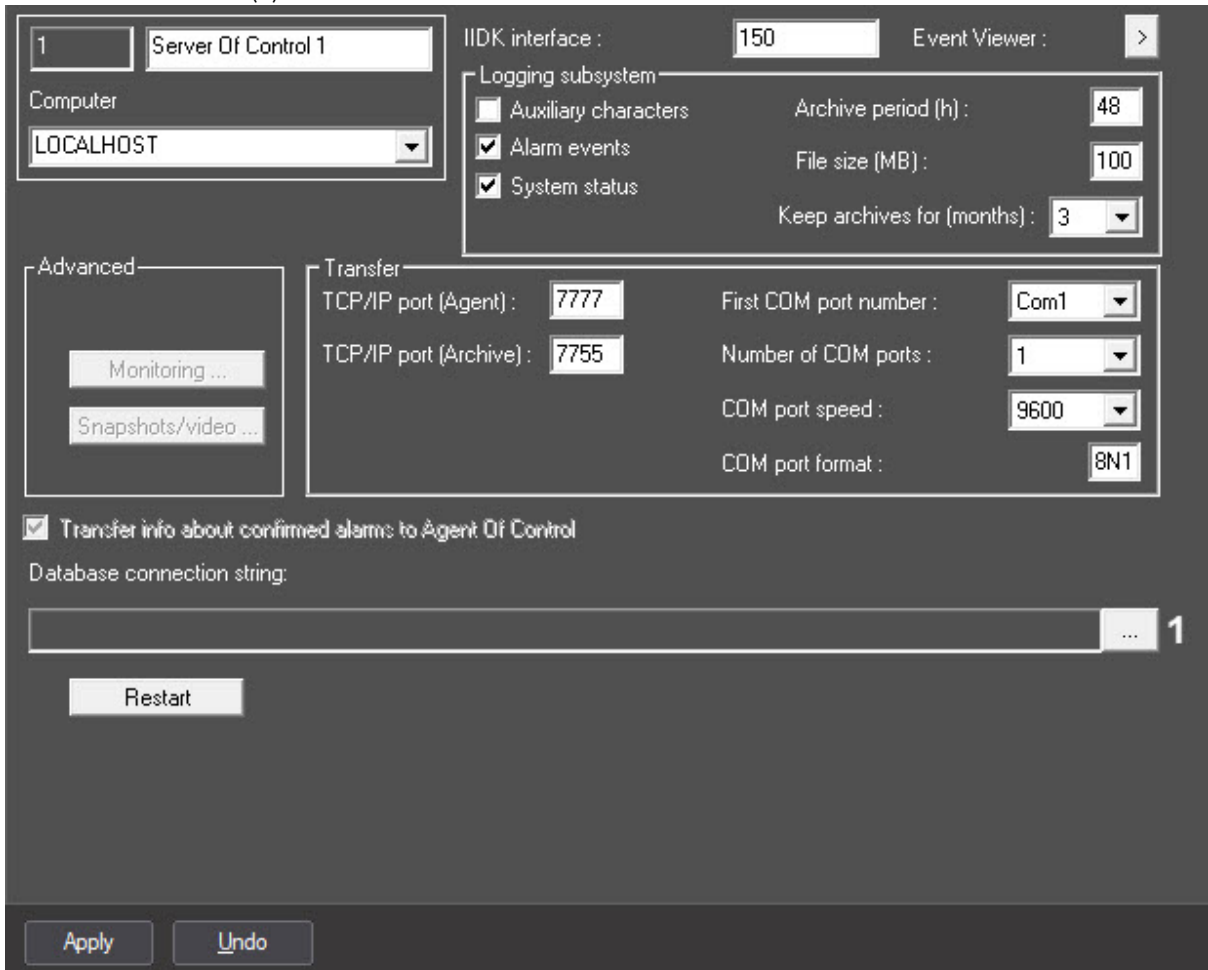

The screenshot shows the configuration window for 'Server Of Control 1'. It includes the following sections and fields:


- General:** IDDK interface: 150, Event Viewer: >
- Logging subsystem:**
 - Auxiliary characters
 - Alarm events
 - System status
 - Archive period (h): 48
 - File size (MB): 100
 - Keep archives for (months): 3
- Transfer:**
 - TCP/IP port (Agent): 7777
 - TCP/IP port (Archive): 7755
 - First COM port number: Com1
 - Number of COM ports: 1
 - COM port speed: 9600
 - COM port format: 8N1
- Transfer info about confirmed alarms to Agent Of Control
- Database connection string: [Empty field with '...' button]
- Restart button
- Apply and Undo buttons at the bottom.

3. The **Data Link Properties** window opens. Configure the connection to the remote *Server of Control* database as follows:


Note

The **Database connection string** parameter is displayed only if the *Server of Control* is configured from another server in a distributed configuration.

- a. Go to the **Provider** tab. Select **Microsoft OLE DB Provider for SQL Server**.

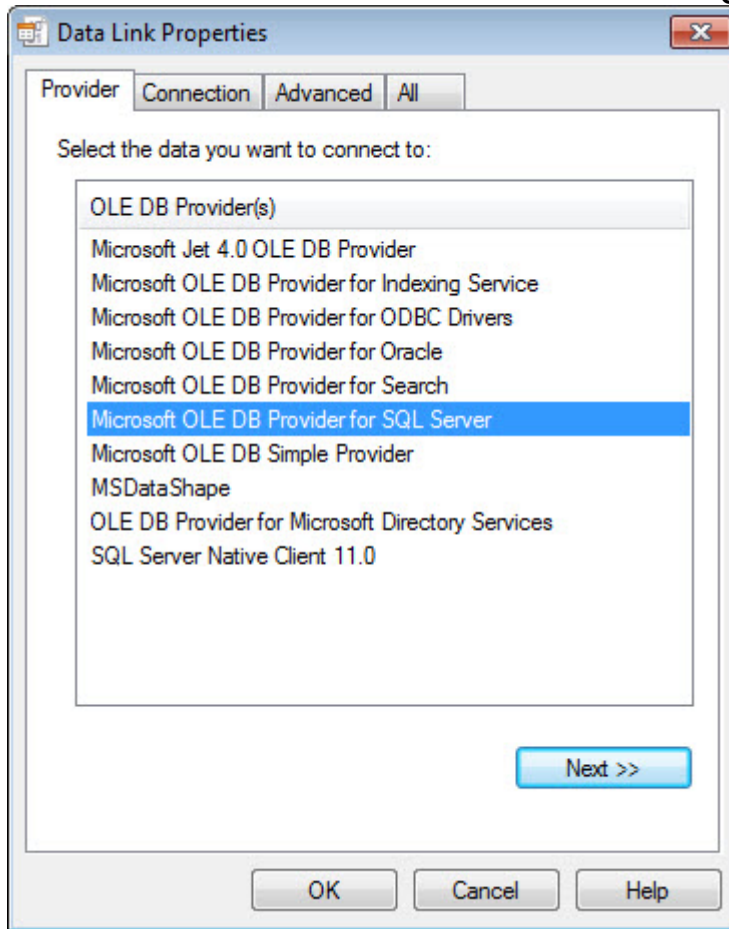

- b. Go to the **Connection** tab. From the **Select or enter a server name** drop-down list, select the name of the database server that stores the *Server of Control* database (1).

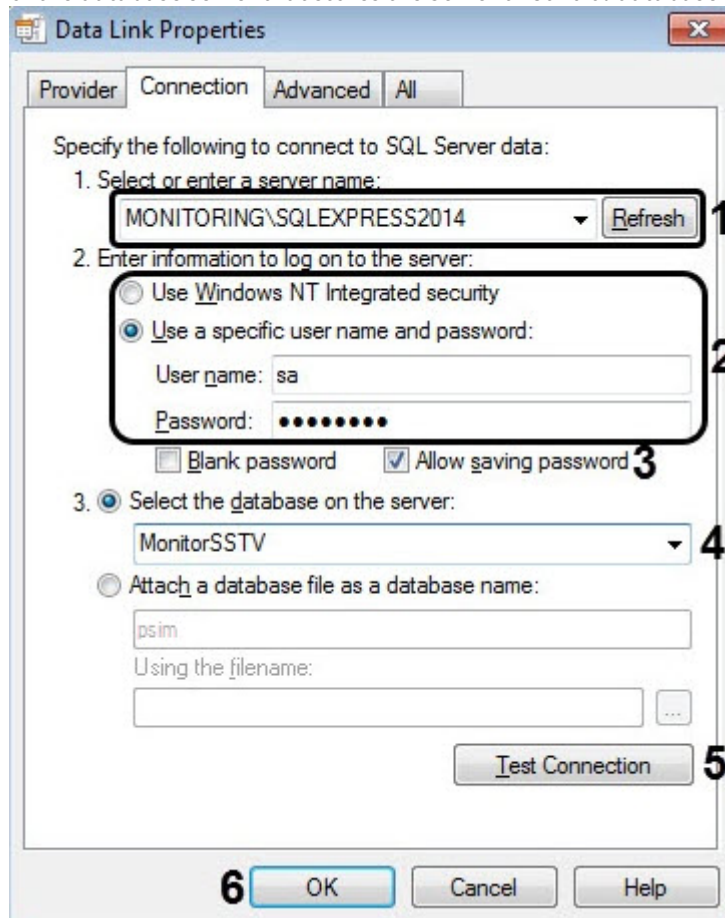

- c. Set the **Enter information to log on to the server** switch to the **Use a specific user name and password** position and enter the name and password to connect to the MS SQL Server (2).
- d. Set the **Allow saving password** checkbox (3).
- e. From the **Select the database on the server** drop-down list, select the name of the *Server of Control* database (**MonitorSSTV** by default) (4).
- f. Click the **Test Connection** button (5). If the connection data is correct, a window with the message "Connection check completed" will be displayed.
- g. Click **OK** (6).

4. The configured string of connection to the *Server of Control* database will be displayed in the text field.

1 Server Of Control 1 IIDK interface : 150 Event Viewer : >

Computer
LOCALHOST

Logging subsystem
 Auxiliary characters Archive period (h) : 48
 Alarm events File size (MB) : 100
 System status Keep archives for (months) : 3

Advanced
Monitoring ...
Snapshots/video ...

Transfer
 TCP/IP port (Agent) : 7777 First COM port number : Com1
 TCP/IP port (Archive) : 7755 Number of COM ports : 1
 COM port speed : 9600
 COM port format : 8N1

Transfer info about confirmed alarms to Agent Of Control

Database connection string:
 Provider=SQLOLEDB.1;Password=***;Persist Security Info=True;User ID=sa;Initial Catalog=MonitorSSTV.Data Sour ...

Restart

Apply Undo

5. As a result, you can start configuring the *Server of Control* (see [Configuring Server of Control](#)).

Configuring the *Server of Control* from another server in a distributed configuration is now complete.

6.10 Sending alarm events via Telegram bot

Configure the sending of alarm events via **Telegram bot** as follows:

1. Go to the settings panel of the **Server Of Control** object created on the basis of the **Computer** object on the **Hardware** tab of the **System settings** dialog box.

2. Click the **Monitoring** button (1).

The screenshot shows the configuration window for the Server of Control. The window is titled "Server Of Control 1" and has a "Computer" dropdown menu set to "LOCALHOST". The "IIDK interface" is set to "150" and the "Event Viewer" is set to ">". The "Logging subsystem" section includes checkboxes for "Auxiliary characters" (unchecked), "Alarm events" (checked), and "System status" (checked). The "Archive period (h)" is set to "48", the "File size (MB)" is set to "100", and "Keep archives for (months)" is set to "3". The "Advanced" section contains two buttons: "Monitoring ..." (highlighted with a red circle and the number 1) and "Snapshots/video ...". The "Transfer" section includes "TCP/IP port (Agent)" set to "7777", "TCP/IP port (Archive)" set to "7755", "First COM port number" set to "Com1", "Number of COM ports" set to "1", "COM port speed" set to "9600", and "COM port format" set to "8N1". A checkbox labeled "Transfer info about confirmed alarms to Agent Of Control" is checked. A "Restart" button is located at the bottom left. At the bottom of the window, there are "Apply" and "Undo" buttons, and a large number "2" is displayed in the bottom left corner.

As a result, the **Monitoring** settings dialog box will open:


3. On the **Events relaying** tab (1), click the **Add** button (2). As a result, the **Event relaying** form will open:

4. From the **Object** drop-down list (1), select the object which events should be sent via **Telegram bot**. The field is empty by default; if you leave it blank, events from all objects will be relayed.
5. From the **Event** drop-down list (2), select an event to send via **Telegram bot**. The field is empty by default; if you leave it blank, all events of the selected object will be relayed.
6. If necessary, fill in the **Filter** field (3). Example: at the **Agent Of Control** object, when describing Monitoring events, two events are assigned to the **Detection tools** button: **Camera disarmed** and **Camera armed**. If you enter **disarmed** in the **Filter** field, then only the **Camera disarmed** event will be relayed to the **Telegram bot**.
7. From the **Telegram bot** drop-down list (4), select the bot via which the events will be relayed.


Note

The **Telegram bot** object should be created and configured beforehand (see [Sending messages via Telegram bot](#)).

8. Set the **Frames** checkbox (5) to relay the JPEG frame linked to the event. When the checkbox is set, two messages will be sent to Telegram: an alarm, and then a frame:

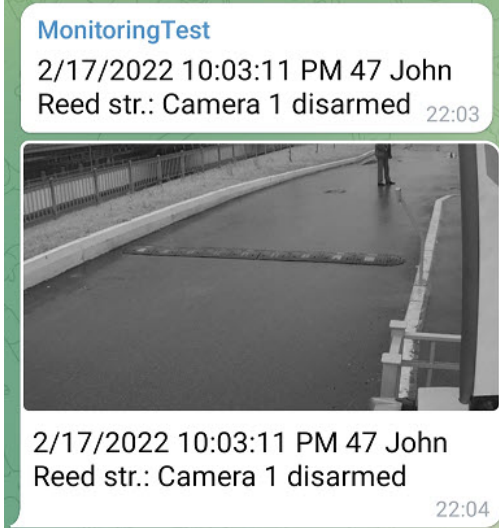


For objects with the specified geocoordinates, a geo-link will be sent in the message:

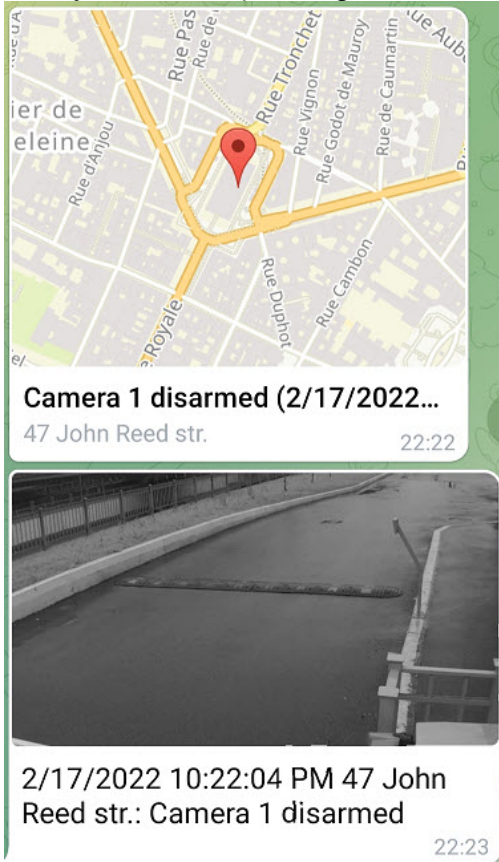


Note

To specify the **Geocoordinates**, go to the settings panel of the **Partition Of Control** object (see [Creating necessary Server Of Control objects](#)) and enter the values in the **Latitude (1)** and **Longitude (2)** fields:

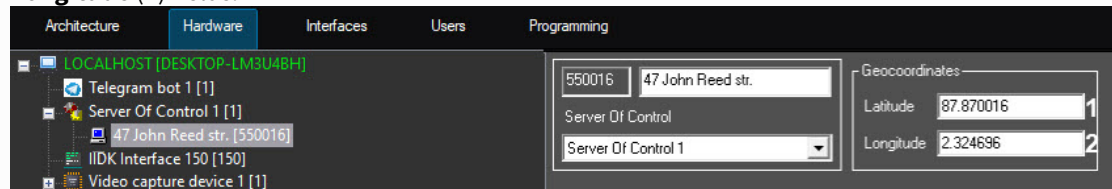

9. Click the **OK** button (6). As a result, the **Event relaying** form will be closed and a new entry will appear in the list in the **Monitoring** settings window:

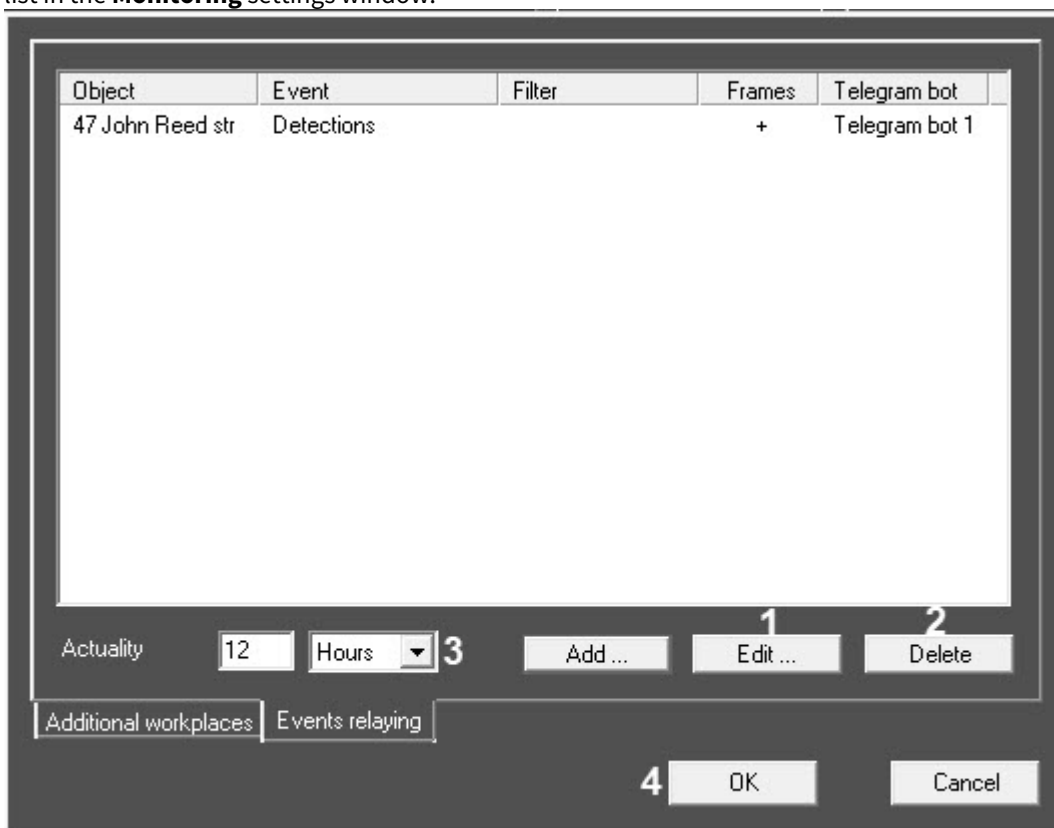

10. In the **Monitoring** settings window, click the **Edit** button (1) to change an existing entry, or the **Delete** button (2) to remove an entry from the list.
11. Fill in the **Actuality** field. To do this, enter a value in the numeric field and select **Hours** or **Minutes** from the drop-down list of measurement units (3). The default value is 12 hours. This setting is used to filter out non-relevant alarms. For example, **Agent Of Control** was disconnected for several days. After the connection is established, the old alarms that occurred during this time will be sent. To prevent old alarms from being relayed to Telegram, you can set their actuality in hours or minutes.
12. Click the **OK** button (4). As a result, the **Monitoring** settings window will be closed and you will return to the settings panel of the **Server Of Control** object.
13. To save the changes, click the **Apply** button (2) on the settings panel of the **Server Of Control** object.

Configuring the sending of alarm messages via the **Telegram bot** is now complete.


7 Configuring Central Server of Control

7.1 General principles of the Central Server of Control software

The CentralNetServer.exe communication module of the *Central Server of Control* (hereinafter referred to as CSC) polls the *Servers of Control* at specified intervals, sending the requests for information about changes in the **MonitorSSTV** database. Each *Server of Control* is requested in parallel in a separate thread. When the *Server of Control* receives such a request, it unloads the latest changes from the **MonitorSSTV** database with the help of the *Agent DB* (MonitorSSTVClient.exe). The CentralNetServer.exe communication module of the CSC receives this data and sends it to the Loader (MonitorSSTVAgent.exe), which then loads this data into the **ServerSSTV** database.

The data between the CSC and the *Servers of Control* is exchanged via FTP protocol, therefore it is necessary to configure the FTP server (see [Configuring the FTP server for the Central Server of Control operation](#)) on the *Server of Control* side.

The general scheme of the *Central Server of Control* software operation is shown in the figure below.

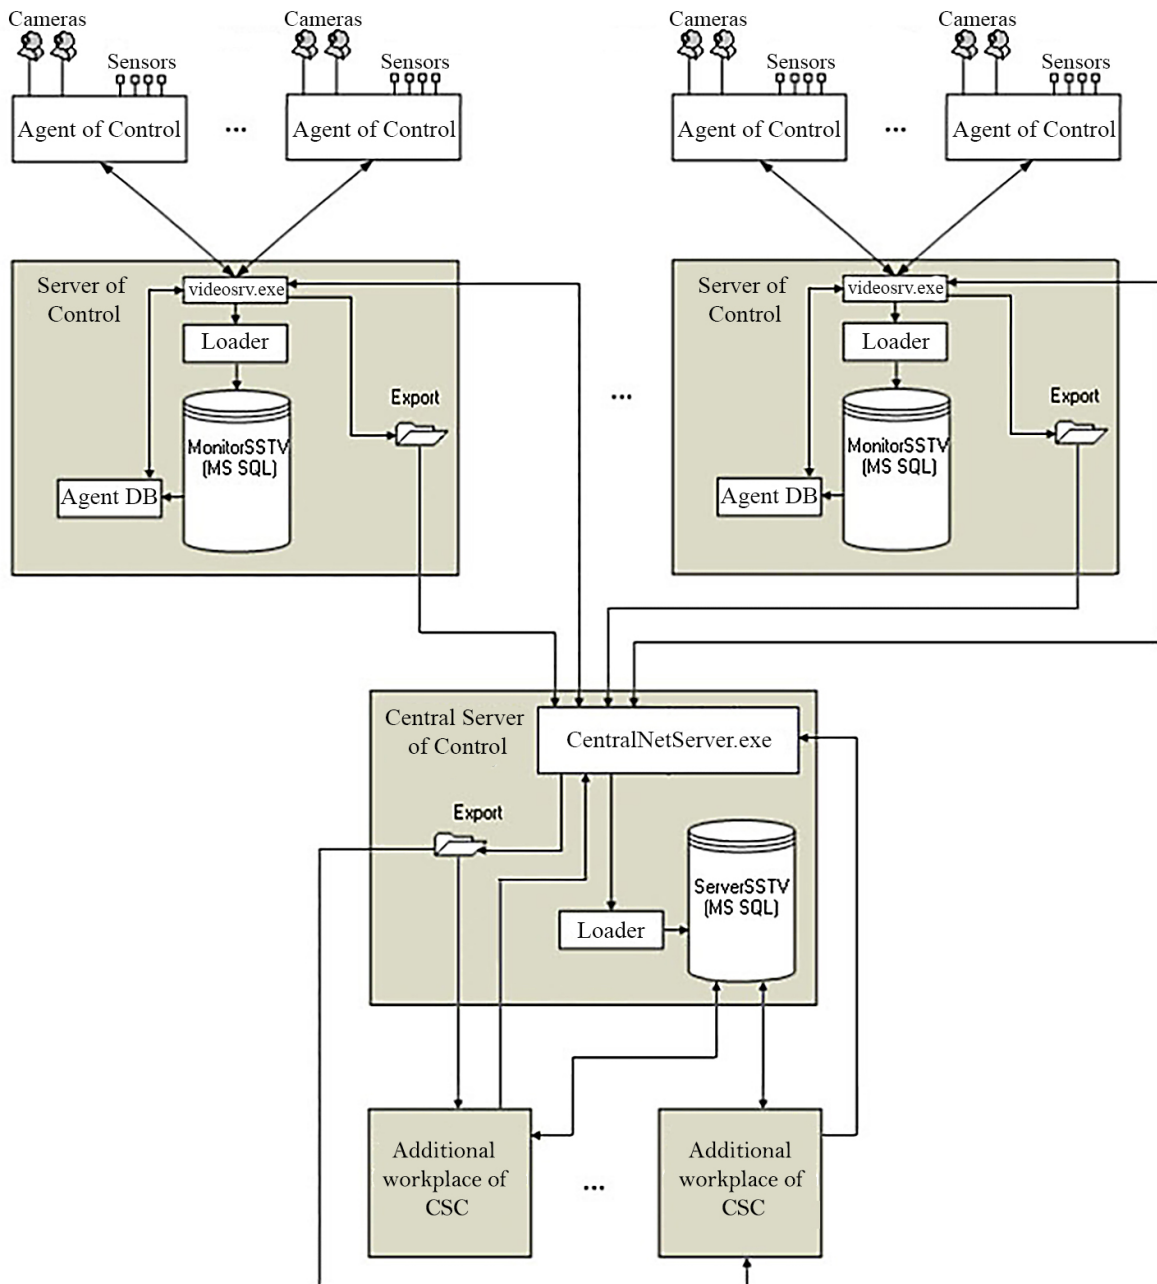

The *Central Server of Control* software provides the same functionality as the *Server of Control* software, but with some restrictions that are listed below.

The main functionality of the *Central Server of Control* software:

- Monitoring of all objects of the video surveillance system, as well as viewing live video and providing the ability to use the **Data gateway** object for this (you can do it in the **Monitoring** interface object).
- Searching for titles and video fragments and, based on the search results, downloading the frames and videos (you can do it in the **Search in archive** interface object).
- Generating the reports on the whole system (you can do it in the **Monitoring reports** interface object).

Restrictions of the *Central Server of Control* software:

- Demo mode is not supported.
- Alarms and errors received from the *Servers of Control* do not appear immediately on the CSC, but with the specified polling frequency of the Servers (see the **PeriodRequestOfStatistic** registry key in [Advanced settings of the Central Server of Control](#)).
- The CSC operator cannot confirm alarms in the **Monitoring** interface object. There are no **Confirm selected**, **Confirm**, and **Confirm all** buttons in the **Reaction to alarm** window.
- The toolbar of the **Monitoring** interface object has no **Force error closing** and **Show closed errors** buttons.
- The **Owner** directory cannot be edited. This directory is automatically filled with the *Servers of Control* names with which the CSC works. The filtering by the *Servers of Control* is supported. Also, the information from the **Owner** directory filled out on the *Server of Control* side is not transmitted to the CSC.
- The special operation mode joint with *Auto PSIM* is not supported (see [Configuring special operation mode joint with Auto PSIM](#)). If this mode is used in the *Server of Control*, then the information from the corresponding tables is not transmitted to the CSC.
- The special operation mode joint with *ACFA PSIM* is not supported (see [Configuring the special mode of Monitoring operation with ACFA PSIM](#)).
- The commands for *Agents of Control* are not supported (see [Sample script for processing Server of Control command on Agent of Control](#)).
- The video data received with the alarm is not displayed. In the **Monitoring** interface object, when right-clicking on an object, the **Video data** item is missing in the context menu.
- The **Search in archive** interface object does not support the automation of downloading videos using the XML files.

7.2 Configuring the FTP server for the Central Server of Control operation

By default, the *Central Server of Control* software works via FTP in a passive mode, and this requires adding the range of ports to which the *Central Server of Control* software will connect in the FTP server settings. It is possible to switch to the active mode. To do this, it is necessary to set the **0** value for the **PassiveModeForFTP** registry key (for details, see [Registry keys reference guide](#)).

The FTP server for the *Central Server of Control* operation should be configured on the side of each *Server of Control* as follows:


1. Create a user with administrator rights in the system.

 **Note**


The password validity period for this user should not be limited in time.

2. If IIS is not installed, install it:
 - a. Open the **Control Panel** → **Programs and Features** → **Turn Windows Features on or off**.

- b. In the **IIS Services** section, select the checkboxes next to the **FTP Service** and **IIS Management Console** components.

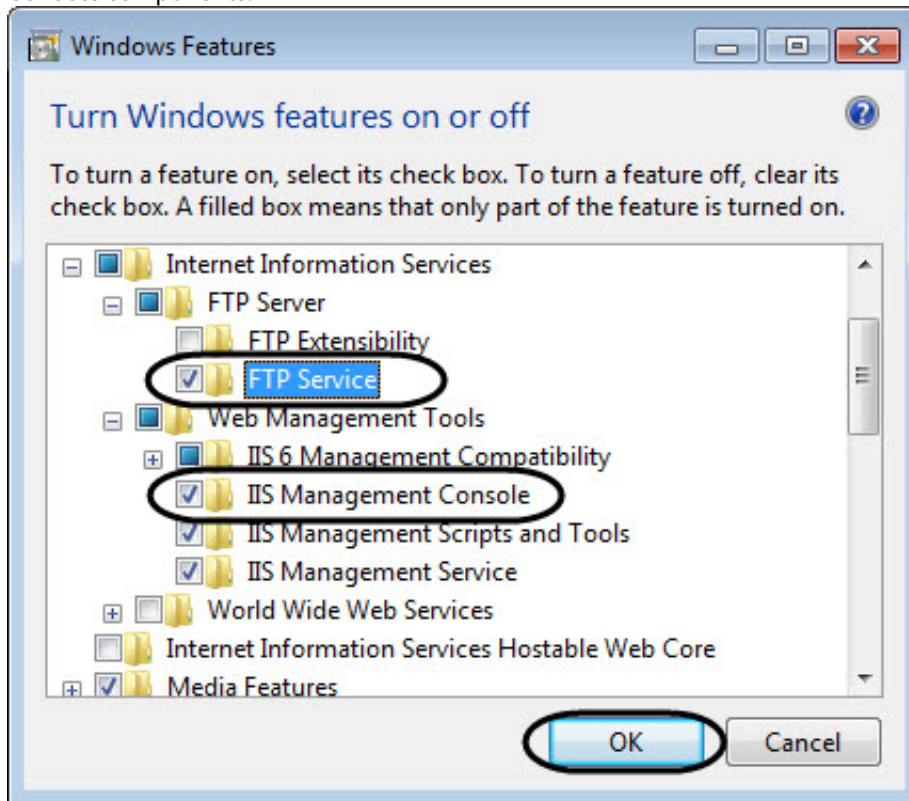

- c. Click **OK**.
3. Open **Computer Management** and in the **Services and Applications** section (1), select **IIS Manager** (2).
 - a. In the **Connections** area, select the **Sites** folder (3), and then in the **Actions** area, click the **Add FTP Site...** link (4). As a result, the **Add FTP Site** window appears.

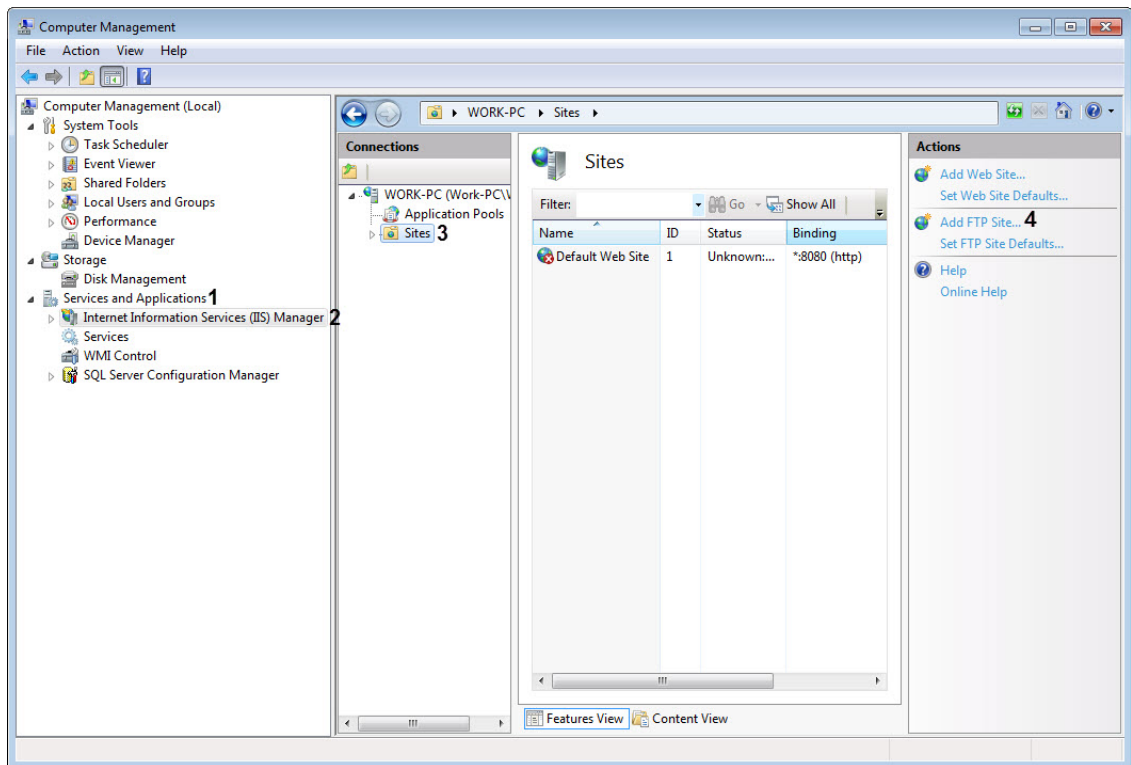

- b. In the **FTP site name** field (5), enter the name of the FTP site.
- c. In the **Physical path** field (6), or using the button, specify the path to the FTP directory. By default, the FTP directory is located at <Axxon PSIM installation directory>\Vhost\DATA\FTP\. You can change this directory using the **FtpPath** registry key (for details, see [Registry keys reference guide](#)).

Note

To increase the performance of data exchange, it is recommended that the export directory (see [Specifying the export directory](#)) and the FTP directory are located on the same disk.


The screenshot shows the 'Add FTP Site' dialog box with the 'Site Information' tab selected. The 'FTP site name' is 'FTP-Сервер' with a '5' next to it. The 'Content Directory' section has a 'Physical path' of 'C:\Program Files (x86)\Axxon PSIM\Vhost\DATA\FTP' with a '6' next to it and a browse button. At the bottom are 'Previous', 'Next', 'Finish', and 'Cancel' buttons.

- d. Click **Next**.
- e. Configure the binding and SSL settings as shown in the figure below.

The screenshot shows the 'Add FTP Site' dialog box with the 'Binding and SSL Settings' tab selected. Under 'Binding', 'IP Address' is 'All Unassigned' and 'Port' is '21'. The 'Enable Virtual Host Names' checkbox is unchecked. Under 'Start FTP site automatically', the checkbox is checked. Under 'SSL', 'No SSL' is selected. The 'SSL Certificate' is 'Not Selected' with a 'View...' button. At the bottom are 'Previous', 'Next', 'Finish', and 'Cancel' buttons.

- f. Click **Next**.

- g. Configure the authentication and authorization as shown in the figure below. It is necessary to specify the user created in step 1 as the authorized user.

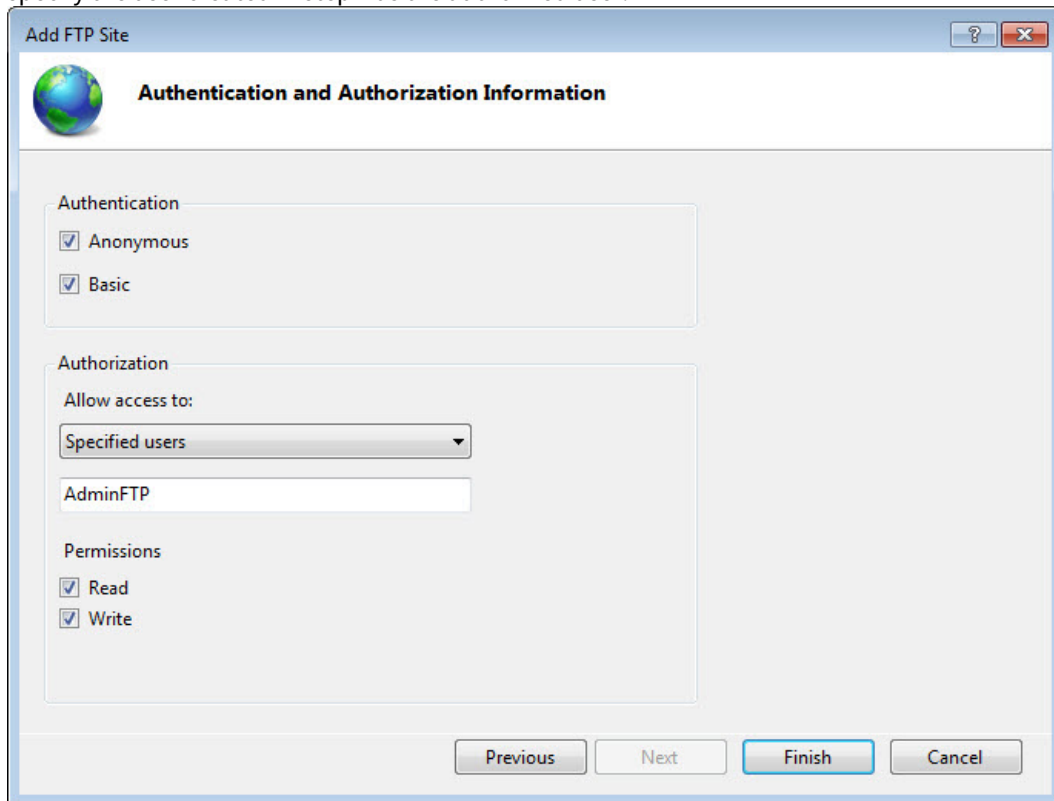

- h. Click **Finish**.


Configuring the FTP server for the *Central Server of Control* software operation is complete.

7.3 Creating the Central Server Of Control object

Create the **Central Server Of Control** object in the hardware tree as follows:

1. Go to the **Hardware** tab of the **System settings** dialog box.

- On the basis of the **Computer** object, create the **Central Server Of Control** object.

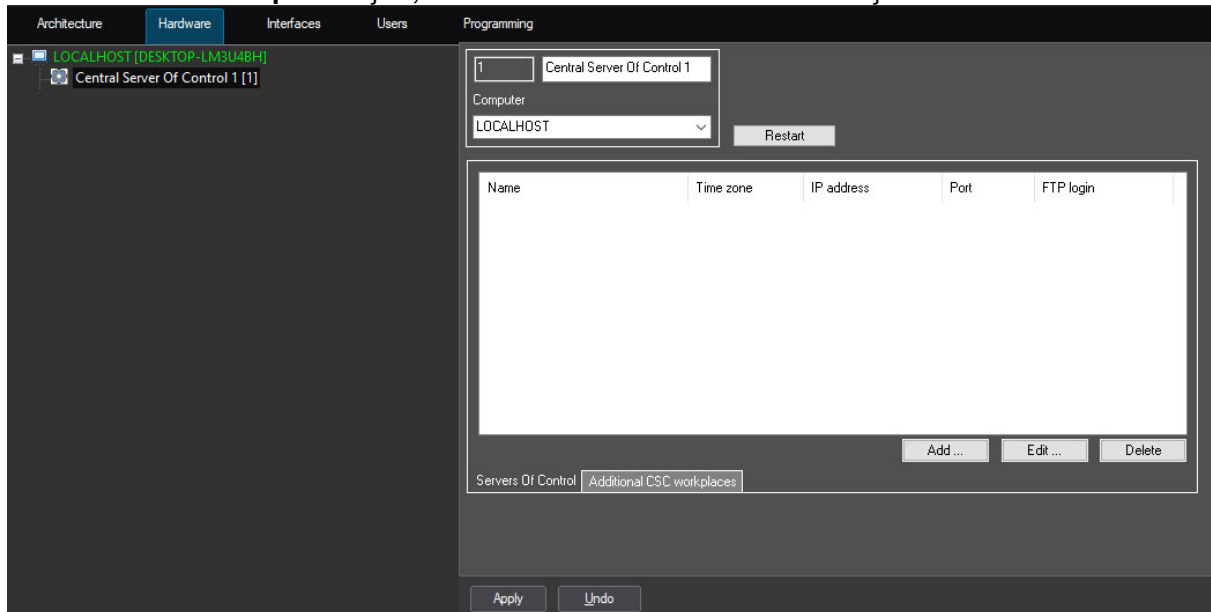


Creation of the **Central Server Of Control** object is completed.

7.4 Configuring the Servers of Control tracking

7.4.1 Adding the Server Of Control

To add the *Server Of Control*, do the following:

- Go to the settings panel of the **Central Server Of Control** object.

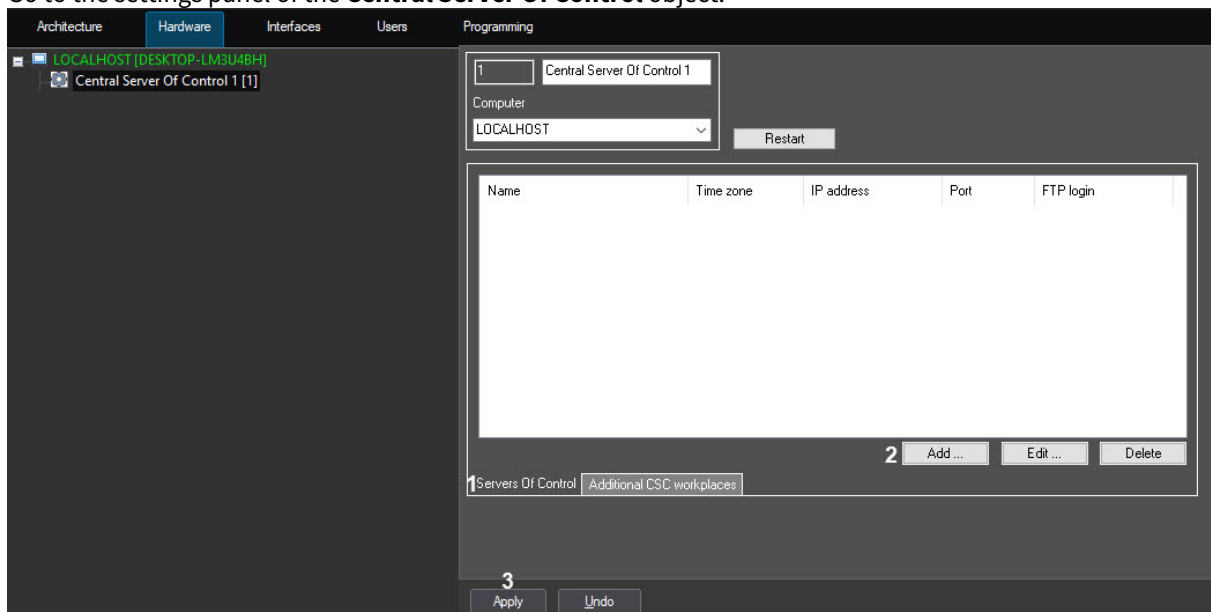

- On the **Servers Of Control** tab (1), click the **Add** button (2).
- In the **Server Of Control** window that appears, do the following:

- a. In the **Name** field (1), enter the name of the *Server Of Control*.

- b. From the **Time zone** drop-down list (2), select the value corresponding to the time zone difference between the Server that should be tracked and the Server on which the *Central Server Of Control* is installed.

Note

For example, if the *Central Server Of Control* is installed on the Server in Oslo, and the Server that should be tracked is located in London, then it is necessary to select the time zone **-1**.

- c. In the **IP address** field (3), specify the IP address of the *Server Of Control*.
- d. In the **Port** field (4), specify the connection port of the *Server Of Control*.
- e. In the **FTP login** field (5), enter the username with administrator rights to connect to the FTP Server. This server will be used for exchanging the data between the *Central Server Of Control* and the *Server Of Control* (see [Configuring the FTP server for the Central Server of Control operation](#)).
- f. In the **FTP password** field (6), enter the password of the user with administrator rights to connect to the FTP server.
- g. In the **Confirmation of FTP password** field (7), re-enter the password for connecting to the FTP Server.
- h. Click the **OK** button (8).

- As a result, the specified *Server Of Control* will be added to the list, and the *Central Server Of Control* will restart automatically.

Name	Time zone	IP address	Port	FTP login
Server Of Control 1	0	101.101.10.10	7755	ftlogin


- To add other *Servers Of Control*, repeat steps 2-3.
- Click the **Apply** button (3).

The *Server Of Control* is added.


7.4.2 Editing the Server Of Control

To edit the *Server Of Control*, do the following:

1. Go to the settings panel of the **Central Server Of Control** object.

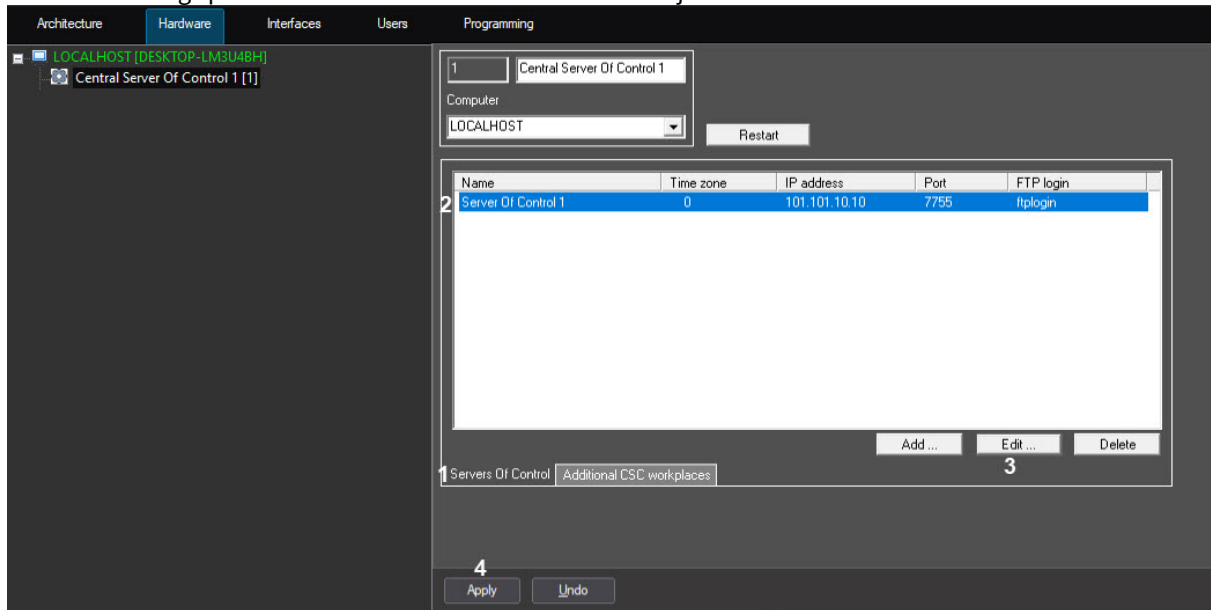

2. On the **Servers Of Control** tab (1), select the *Server Of Control* that should be edited (2), and click the **Edit** button (3).
3. As a result, the **Server Of Control** window will be displayed. Make the necessary changes (for details, see [Adding the Server Of Control](#)).

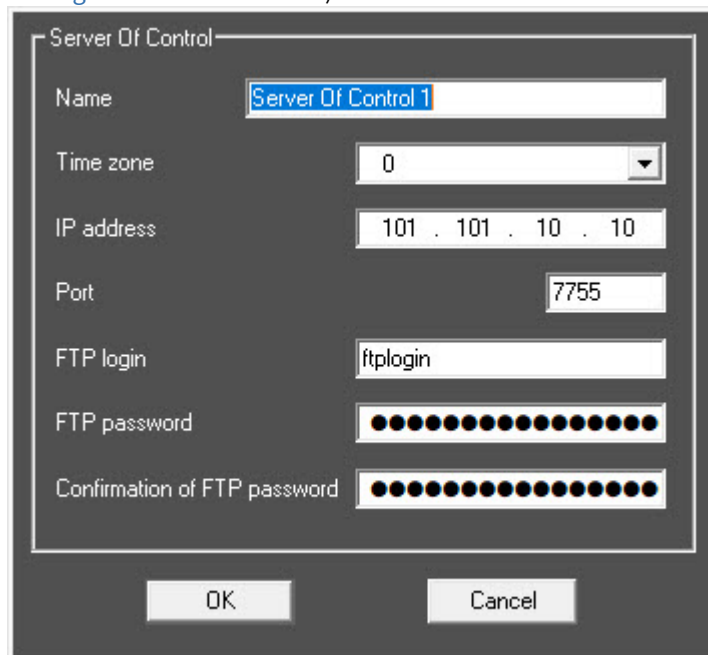


4. Click the **OK** button.
5. Click the **Apply** button (4).

The *Server Of Control* is edited.


7.4.3 Deleting the Server Of Control

To delete the *Server Of Control*, do the following:

1. Go to the settings panel of the **Central Server Of Control** object.

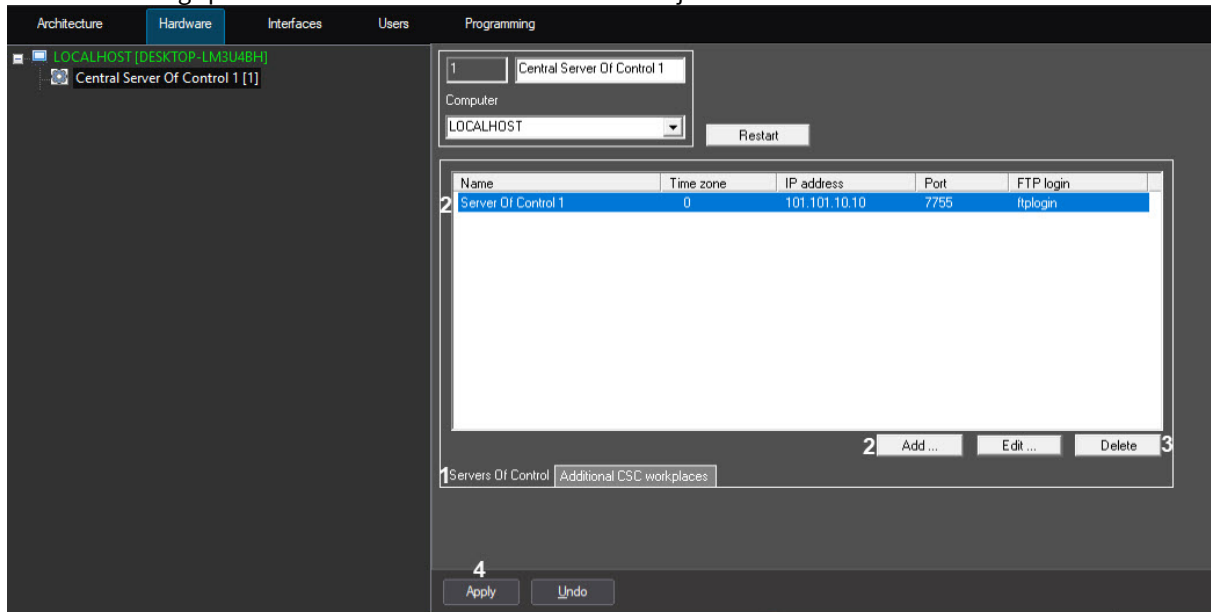

2. On the **Servers Of Control** tab (1), select the *Server Of Control* that should be deleted (2), and click the **Delete** button (3).
3. As a result, a confirmation window will open. Confirm the deletion of the selected *Server Of Control* by clicking the **Yes** button.

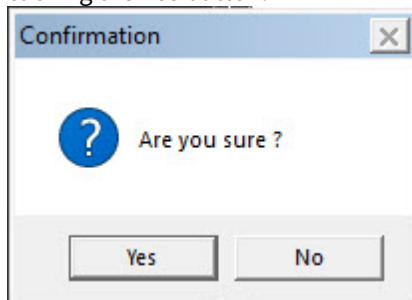

4. Click the **Apply** button (4).

The *Server Of Control* is deleted.


7.5 Configuring the Additional workplace of CSC connection rights to the Central Server of Control

7.5.1 Adding the Additional workplace of CSC


For the *Additional workplace of CSC* software to work, it is necessary to add the *Additional workplaces of CSC* to the *Central Server Of Control*, and specify the computer name and the client code for each of them.

To add the *Additional workplace of CSC*, do the following:

1. Go to the settings panel of the **Central Server Of Control** object.

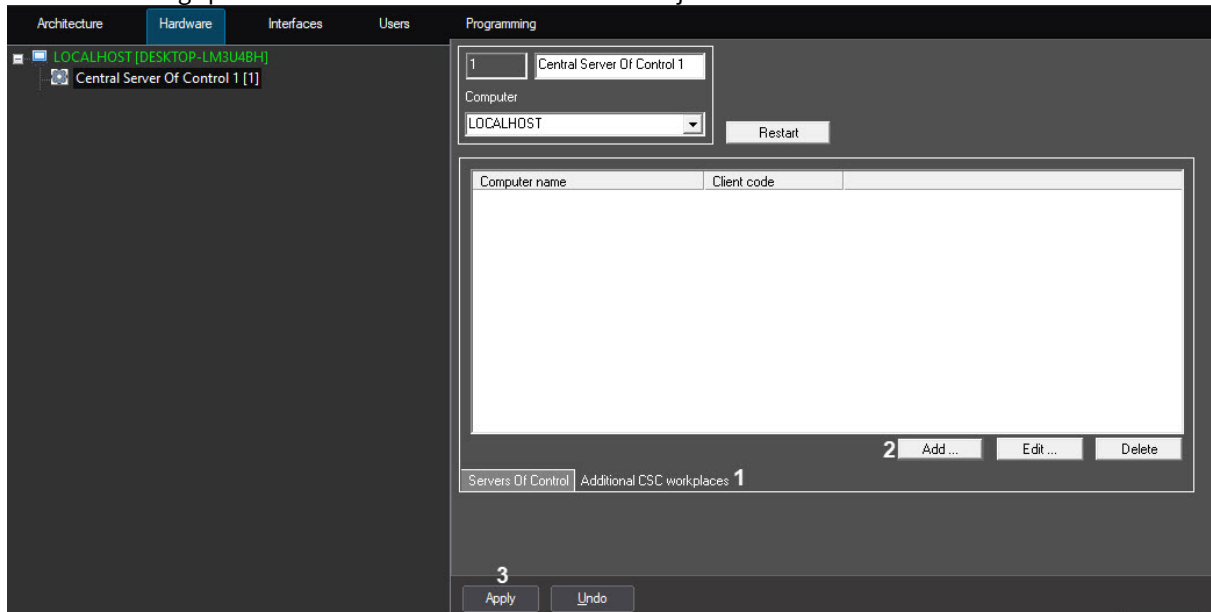

2. On the **Additional CSC workplaces** tab (1), click the **Add** button (2).
3. In the **Additional CSC workplace** window that appears, do the following:
 - a. In the **Computer name** field (1), enter the computer name on which the *Additional workplace of CSC* software is installed.

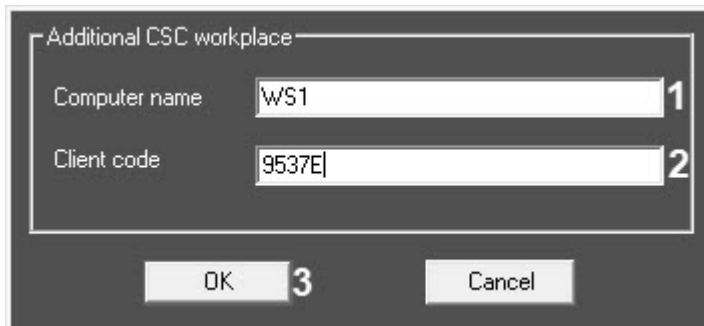

- b. In the **Client code** field (2), specify the Client code that is linked with the computer hardware (for details, see [List of Additional workplaces](#)).
- c. Click the **OK** button (3).

- As a result, the specified *Additional workplace of CSC* will be added to the list, and the *Central Server Of Control* will restart automatically.

Computer name	Client code
WS1	9537E


- To add other *Additional workplaces of CSC*, repeat steps 2-3.
- Click the **Apply** button (3).

The *Additional workplace of CSC* is added.


7.5.2 Editing the Additional workplace of CSC

To edit the *Additional workplace of CSC*, do the following:

1. Go to the settings panel of the **Central Server Of Control** object.

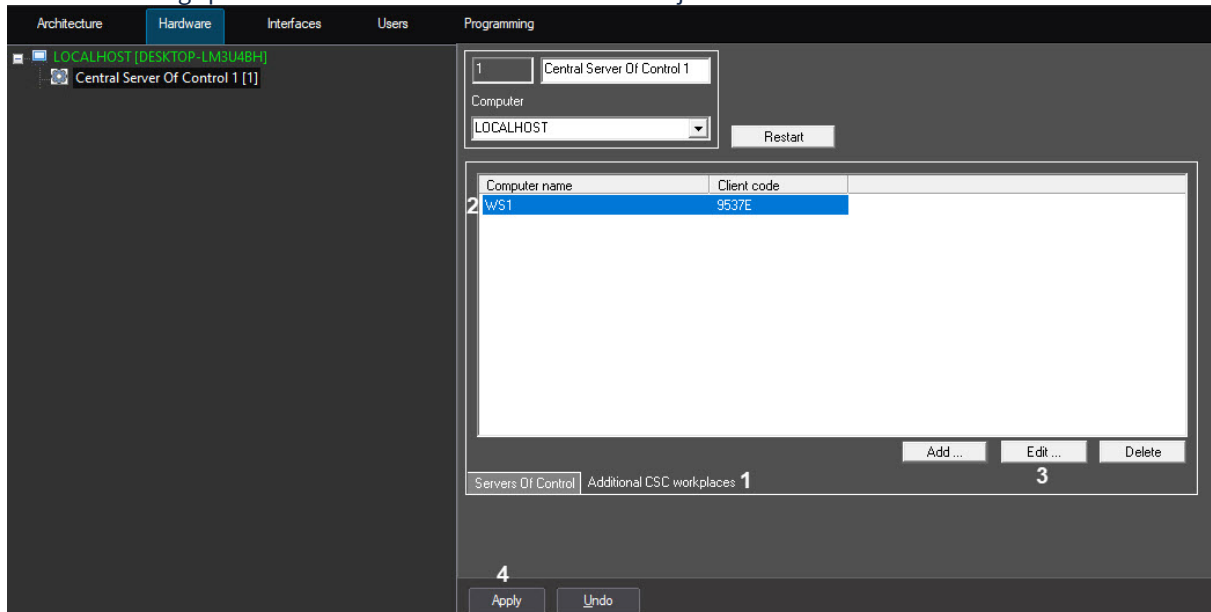

2. On the **Additional CSC workplaces** tab (1), select the *Additional workplace of CSC* which should be edited (2), and click the **Edit** button (3).
3. As a result, the **Additional CSC workplace** window will be displayed where it is necessary to make the corresponding changes (for details, see [Adding the Additional workplace of CSC](#)).

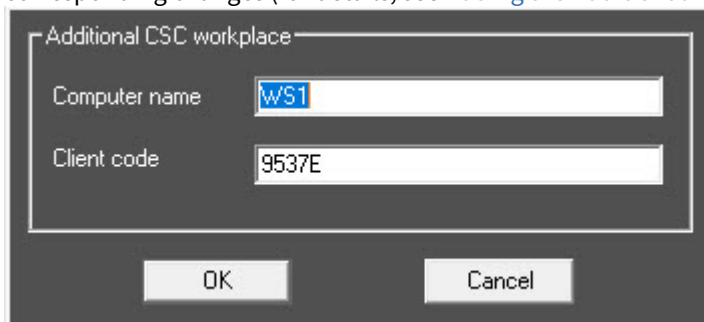


4. Click the **Apply** (4) button.

The *Additional workplace of CSC* is edited.


7.5.3 Deleting the Additional workplace of CSC

To delete the *Additional workplace of CSC*, do the following:

1. Go to the settings panel of the **Central Server Of Control** object.

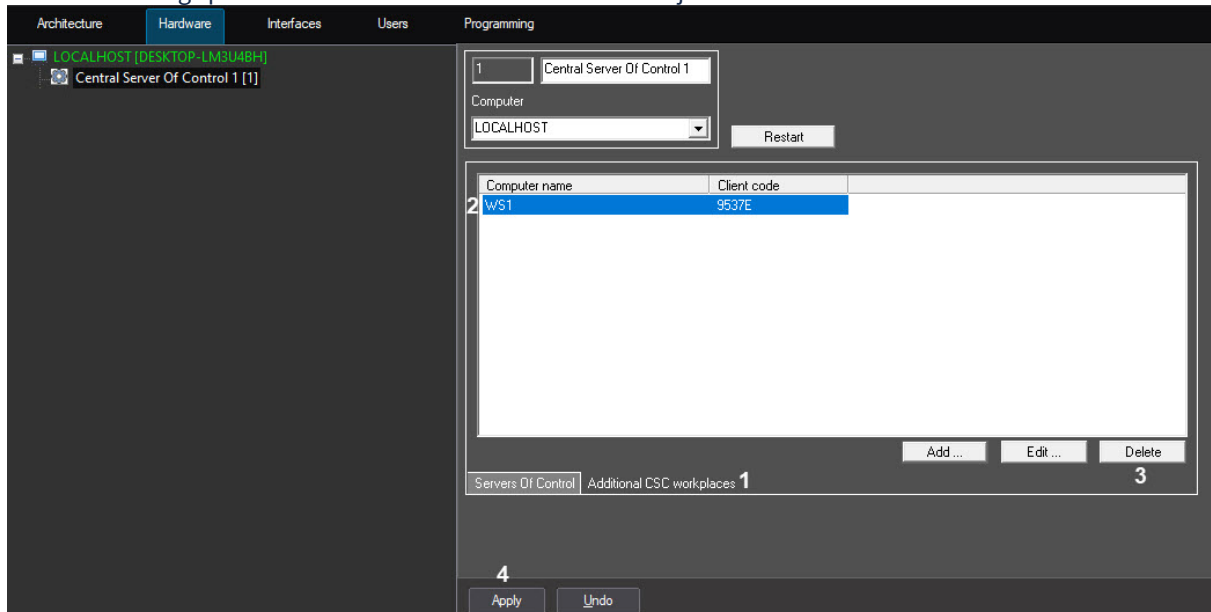

2. On the **Additional CSC workplaces** tab (1), select the *Additional workplace of CSC* which should be deleted (2), and click the **Delete** button (3).
3. As a result, the **Additional CSC workplace** window will be displayed where it is necessary to click the **Yes** button to confirm the deletion of the selected *Additional workplace of CSC*.

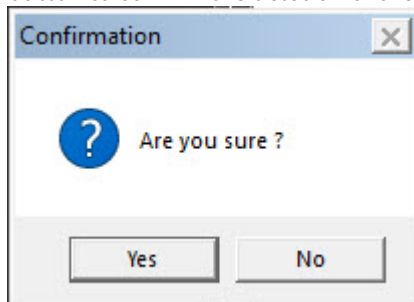

4. Click the **Apply** (4) button.

The *Additional workplace of CSC* is deleted.

7.6 Advanced settings of the Central Server of Control

Note

The registry keys reference guide can be found in the [Registry keys reference guide](#), for more information about working with the registry, see [Working with Windows OS registry](#).

You can apply the advanced settings of the *Central Server of Control* using the following registry keys:

1. To change the polling period of *Servers of Control* statistics, it is necessary to specify the corresponding value in minutes for the **PeriodRequestOfStatistic** registry key.
2. To change the archive period of the CentralNetServer.log log file which belongs to the CentralNetServer.exe communication module, it is necessary to specify the corresponding value in hours for the **LogArchPeriod** registry key.

3. To change the maximum size of the CentralNetServer.log log file which belongs to the CentralNetServer.exe communication module at which it begins to archive ignoring the **LogArchPeriod** parameter, it is necessary to specify the corresponding value in megabytes for the **LogMaxSize** registry key.
4. To change the archive retention period of the CentralNetServer.log log files which belong to the CentralNetServer.exe communication module, it is necessary to specify the corresponding value in months for the **LogArchDelPeriod** registry key. When the retention period is exceeded, the archives are removed.
5. To change the data retention period of closed errors and alarms in the **ServerSSTV** DB, it is necessary to specify the corresponding value in months for the **KeepDB** registry key. When the retention period is exceeded, the data are removed.
6. By default, the *Central Server of Control* requests a complete package of statistics from all *Servers of Control* only once, when it first connects to the *Servers of Control*.
 - To execute a request for a complete statistics package from a specific *Server of Control* once, it is necessary to activate the **RequestFullStatistic[N]** registry key, where N is the internal identifier of the *Server of Control* object. The request will be executed when the CentralNetServer.exe communication module is launched, and the value of this key will automatically change to **0**.
 - To request a complete statistics package from all *Servers of Control* every time the CentralNetServer.exe communication module is launched, it is necessary to activate the **RequestFullStatisticOnStartup** registry key.

 **Attention!**

Requesting a complete statistics package is a resource-intensive operation. It is only necessary to activate the keys request a complete statistics package if absolutely necessary.

Applying the advanced settings of the *Central Server of Control* is completed.

7.7 Working with Central Server Of Control without Windows administration rights

To allow the user not added to the Administrators group in the Windows operating system to work correctly with *Central Server Of Control*, make sure the following conditions are fulfilled:

1. The user must be given full access to the registry key:
 - For a 32-bit system: HKEY_LOCAL_MACHINE\Software\BitSoft
 - For a 64-bit system: HKEY_LOCAL_MACHINE\Software\Wow6432Node\BitSoft
2. The user must be granted full rights to the export directory (see [Specifying the export directory](#)).

7.8 Configuring the Central Server Of Control from another server in a distributed configuration

To configure the *Central Server Of Control* from another server in a distributed configuration, do the following:

1. Go to the settings panel of the **Central Server Of Control** object.

1 Central Server Of Control 1

Computer
VSERVER

Database connection string


Restart

Name	Time zone	IP address	Port	FTP login
------	-----------	------------	------	-----------

Add ... Edit ... Delete

Servers Of Control Additional CSC workplaces


Apply Undo

2. Click the  button (1). The **Data Link Properties** window opens. Configure the connection to the remote *Central Server Of Control* database as follows:


 **Note**

The **Database connection string** parameter is displayed only if the *Central Server Of Control* is configured from another server in a distributed configuration.

- a. Go to the **Provider** tab. Select **Microsoft OLE DB Provider for SQL Server**.

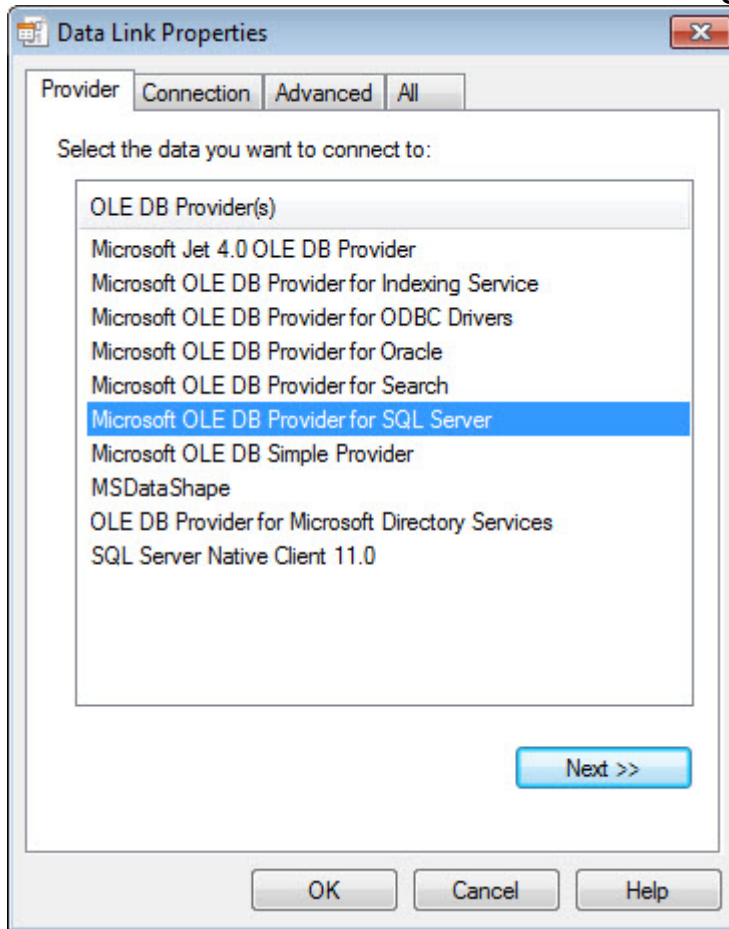

- b. Go to the **Connection** tab. From the **Select or enter a server name** drop-down list, select the name of the database server that stores the *Central Server Of Control* database (1).

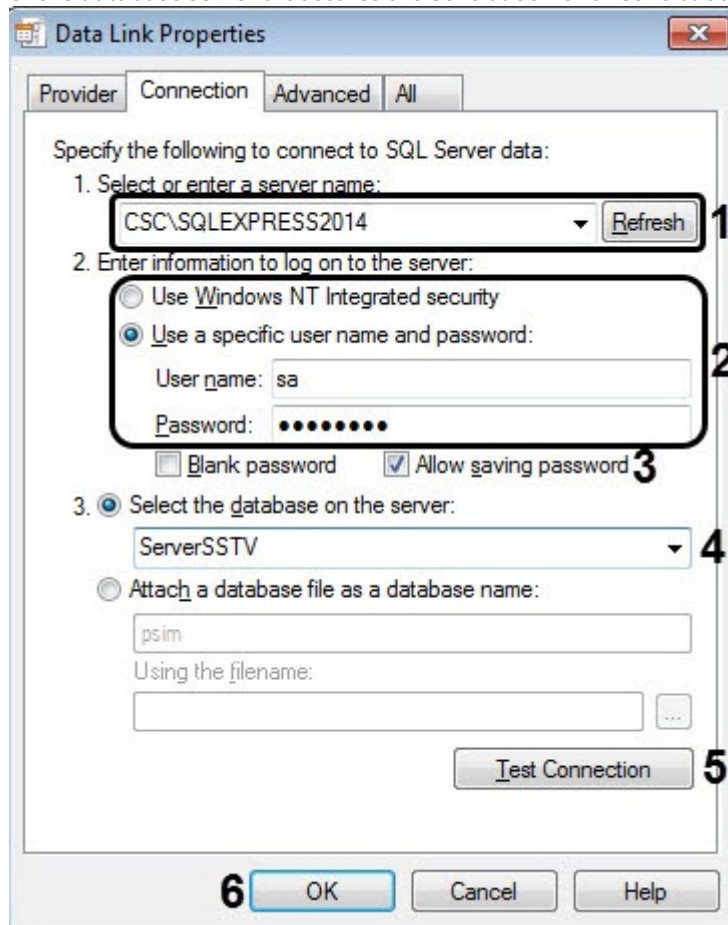

- c. Set the **Enter information to log on to the server** switch to the **Use a specific user name and password** position and enter the name and password to connect to the MS SQL Server (2).
- d. Set the **Allow saving password** checkbox (3).
- e. From the **Select the database on the server** drop-down list, select the name of the *Central Server Of Control* database (ServerSSTV by default) (4).
- f. Click the **Test Connection** button (5). If the connection data is correct, a window with the message "Connection check completed" will be displayed.
- g. Click the **OK** button (6).

- The configured string of connection to the *Central Server Of Control* database will be displayed in the text field (2).

1 Central Server Of Control 1 Database connection string

Computer VSERVER Restart

Provider=SQLOLEDB.1;Password=***;Persist Security Info=True;User ID= ... 2

Name	Time zone	IP address	Port	FTP login
------	-----------	------------	------	-----------

Add ... Edit ... Delete

Servers Of Control Additional CSC workplaces

Apply Undo

- As a result, you can start configuring the *Central Server Of Control* (see [Configuring Central Server of Control](#)). Configuring the *Central Server Of Control* from another server in a distributed configuration is now complete.


8 Configuring Additional workplace and Additional workplace of CSC

8.1 List of Servers of Control/CSC

Additional workplace/Additional workplace of CSC can operate with only one *Server of Control/Central Server of Control* (further named *Server*) at a time. However, the list of Servers can be configured and the active Server can be selected. For this use the *Additional workplace configuration tool*. The tool can be run in one of the following ways:


1. Click **Start -> All Programs -> Axxon PSIM -> Monitoring PSIM -> Additional workplace configuration tool**.
2. Use the *ARMSelector.exe* executable file, located in the <Axxon PSIM installation directory>\Vhost\SYSTEM\ folder.

The tool is shown in the figure.

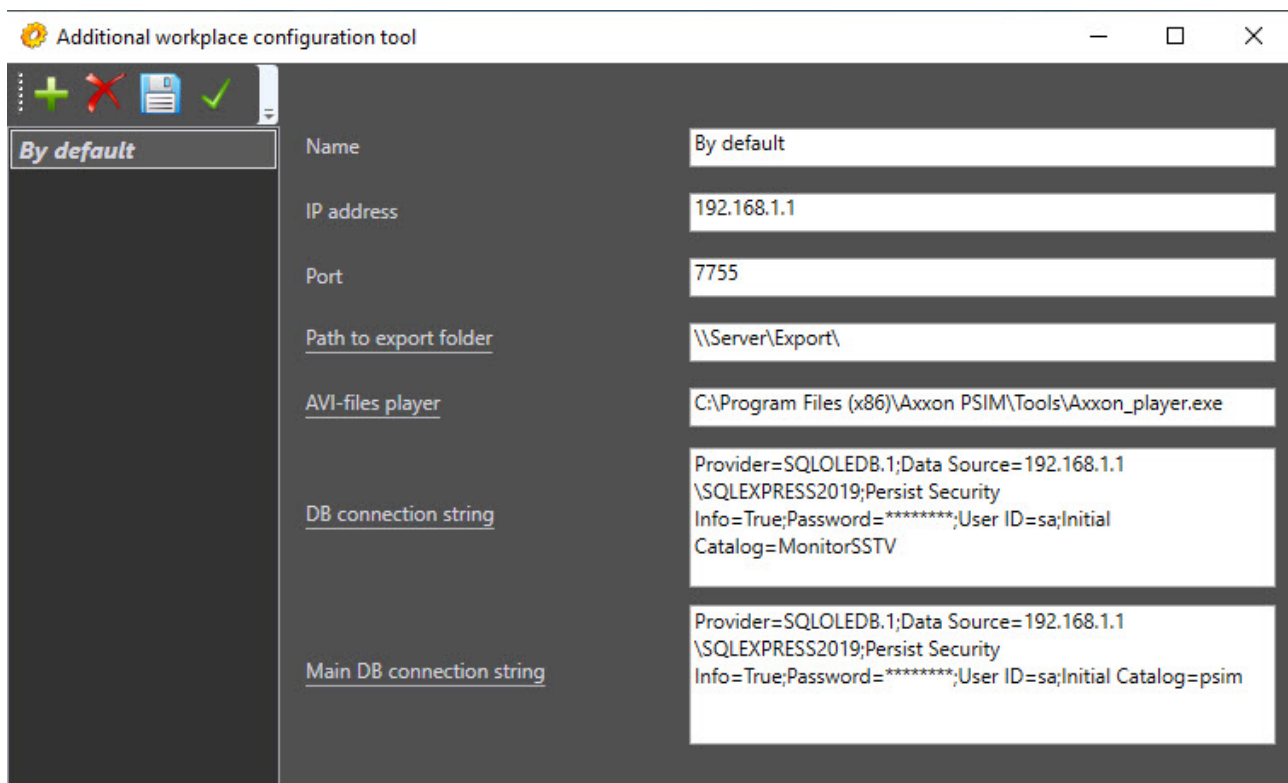

8.1.1 Interface of Additional workplace configuration tool

Interface elements of *Additional workplace configuration tool* are described in the table.

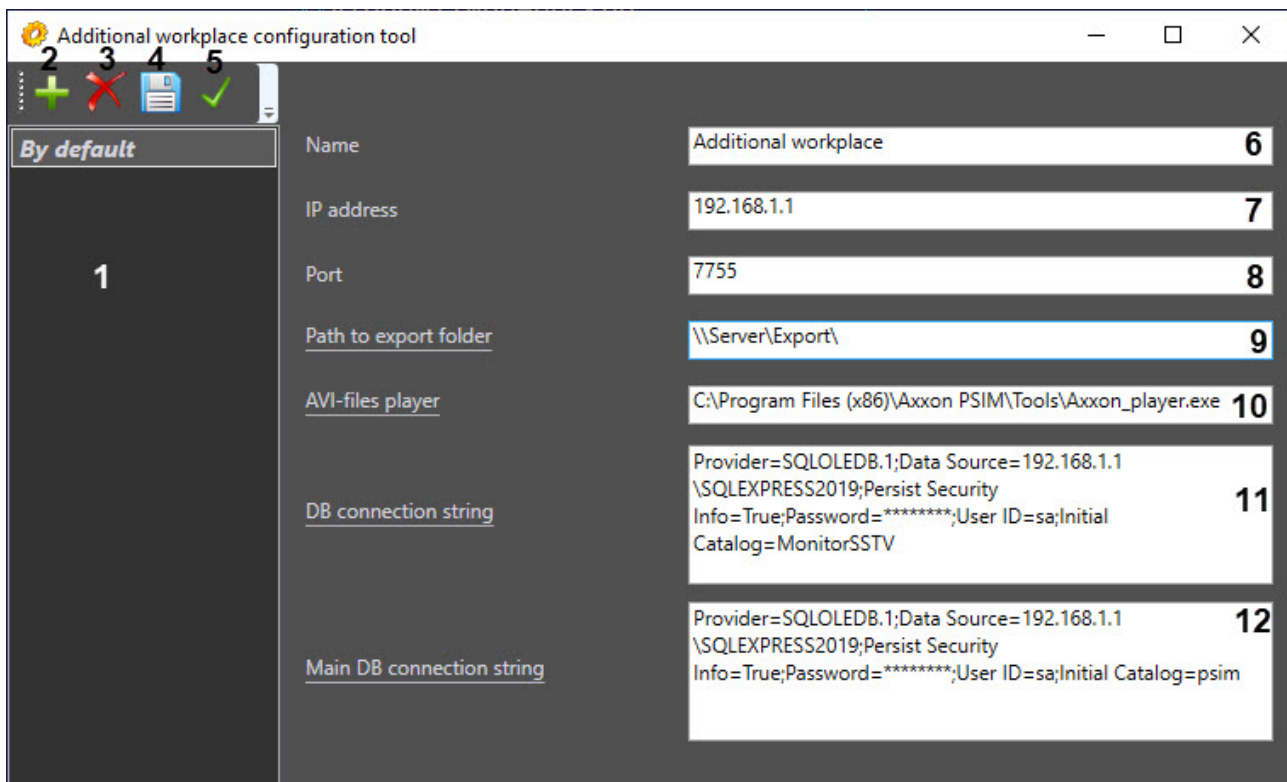

#	Name	Method of setting the parameter value	Default value	Description
1	List of Servers	The Add , Remove and Set as active buttons	By default there is the Server in the list. It is named By default and is created during installation.	Displays the list of existing Servers. An active Server is highlighted in bold.
2	The Add button	Click the button	-	Adding a new Server to the list.
3	The Delete button	Click the button	-	Deleting a selected Server from the list.
4	The Save button	Click the button	-	Saving the changes
5	The Set as active button	Click the button	-	Setting a selected Server as an active one.
6	The Name field	Enter a value in the field	See #1. When a new Server is added to the list it is named New by default.	Setting a name for Server. This name is used only in this tool.

7	The IP address field	Enter a value in the field	127.0.0.1 Important! The value of this parameter is to be changed according to the IP address of the Server.	Setting the IP address to connect to the VideoSrv.exe module (if the <i>Server of Control</i> is added) or CentralNetServer.exe (if the <i>Central Server of Control</i> is added).
8	The Port field	Enter a value in the field	7755	<p>Setting a port to connect to the corresponding communication module VideoSrv.exe/ CentralNetServer.exe.</p> <p>To connect to the VideoSrv.exe module, it is necessary to specify the port that is selected in the TCP/ IP port (Archive) field on the settings panel (see Configuring a connection).</p> <p>To connect to the CentralNetServer.exe module, it is necessary to specify the port that is selected in the IPPort registry key (see Registry keys reference guide, for more information about working with the registry, see Working with Windows OS registry).</p>
9	The Path to export folder field	The Path to export folder link or enter a value in the field	-	Setting a path to the network folder on the Server where there are archive files requested from the <i>Agents of Control</i> .
10	The AVI-files player field	The Path to executable file link or enter a value in the field	-	Setting the path to the executable file of the video player on the <i>Additional workplace/Additional workplace of CSC</i> used to playback the video clips requested from the <i>Agents of Control</i> (see Request for video clips from objects).


1 1	The DB connection string field	The DB connection string link	-	Setting the Server DB connection string. The Data Link Properties box appears when clicking the DB connection string link.
1 2	The Main DB connection string field	The Main DB connection string link	-	Setting the connection string to the base <i>Axxon PSIM</i> DB on the Server. The Data Link Properties box appears when clicking the Main DB connection string link.


8.1.2 Adding Server of Control to the list

By default the Server (named “By default”) is added to Additional workplace configuration right after installation of *Monitoring PSIM* software package. Its settings are the same as those specified during installation (see [Installing Additional workplace software](#) section).

Add a new Server to the list as follows:

1. Run *Additional workplace configuration tool*.

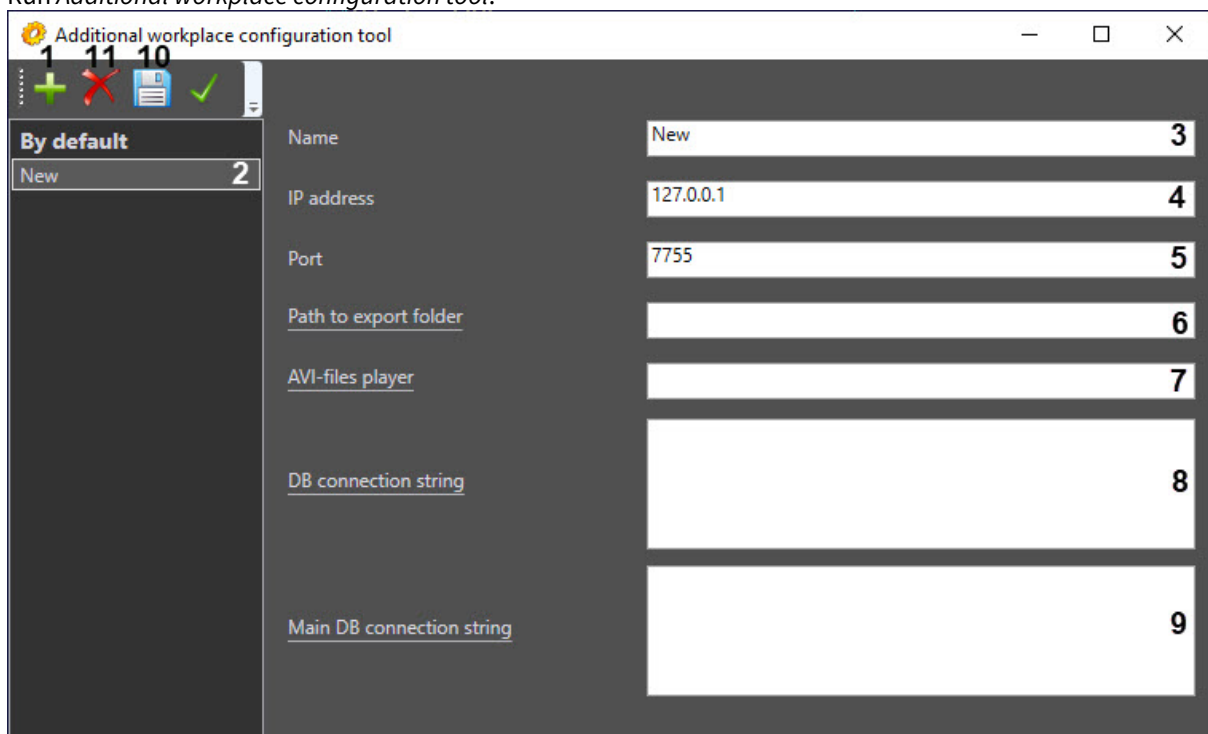

2. Click the  button (1).
3. A new Server named **New** is added to the list (2).
4. Rename the Server if necessary (3).

 **Note.**

This name is used in the Additional workplace configuration tool only.

5. Specify the IP address of computer where the corresponding communication module is run: VideoSrv.exe module (if the *Server of Control* is added) or CentralNetServer.exe (if the *Central Server of Control* is added) (4).
6. Specify the connection port to the VideoSrv.exe/CentralNetServer.exe module (5).


 **Note.**

To connect to the VideoSrv.exe module, it is necessary to specify the port that is selected in the **TCP/IP port (Archive)** field on the settings panel (see [Configuring a connection](#)).


To connect to the CentralNetServer.exe module, it is necessary to specify the port that is selected in the **IPPort** registry key (see [Registry keys reference guide](#)).

7. Specify the path to network folder on the Server where there are archive files requested from the *Agent of Control* (6) (see [Specifying the export directory](#)). A standard **Browse for Folder** dialog box appears when clicking the **Path to export folder** link. Select a required folder.
8. Specify the path to the executable file of the video player on the *Additional workplace/Additional workplace of CSC* used to playback the video clips requested from the *Agents of Control* (see [Request for video clips from objects](#)) (7).
9. Click the **DB connection string** link (8). The **Data Link Properties** box appears. Configure DB connection to remote *Server* as follows:


- a. Go to the **Provider** tab. Select **Microsoft OLE DB Provider for SQL Server**.

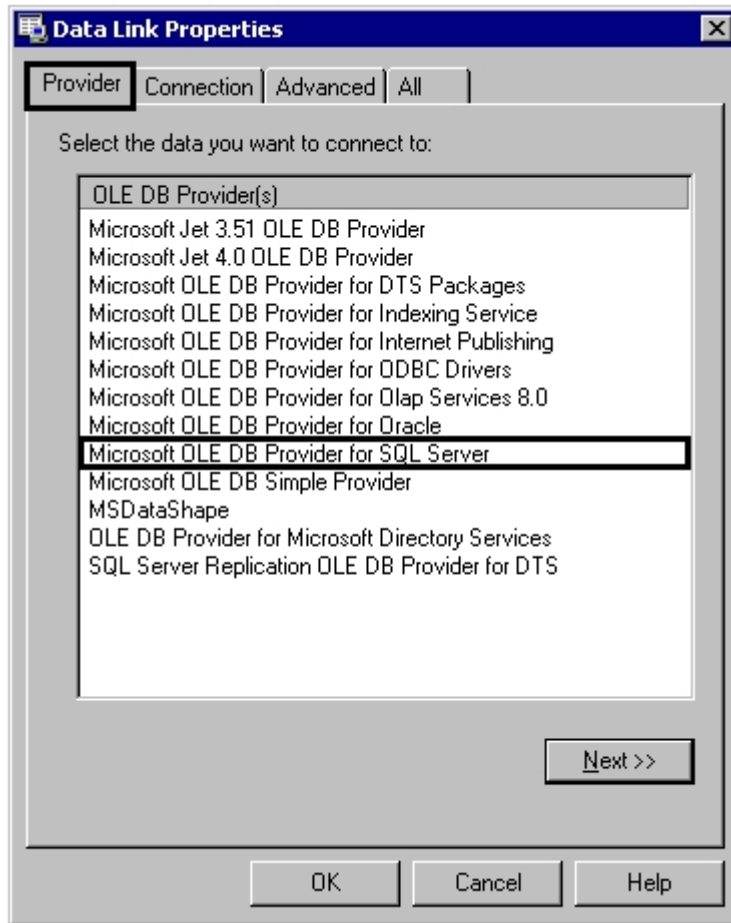

- b. Go to the **Connection** tab.

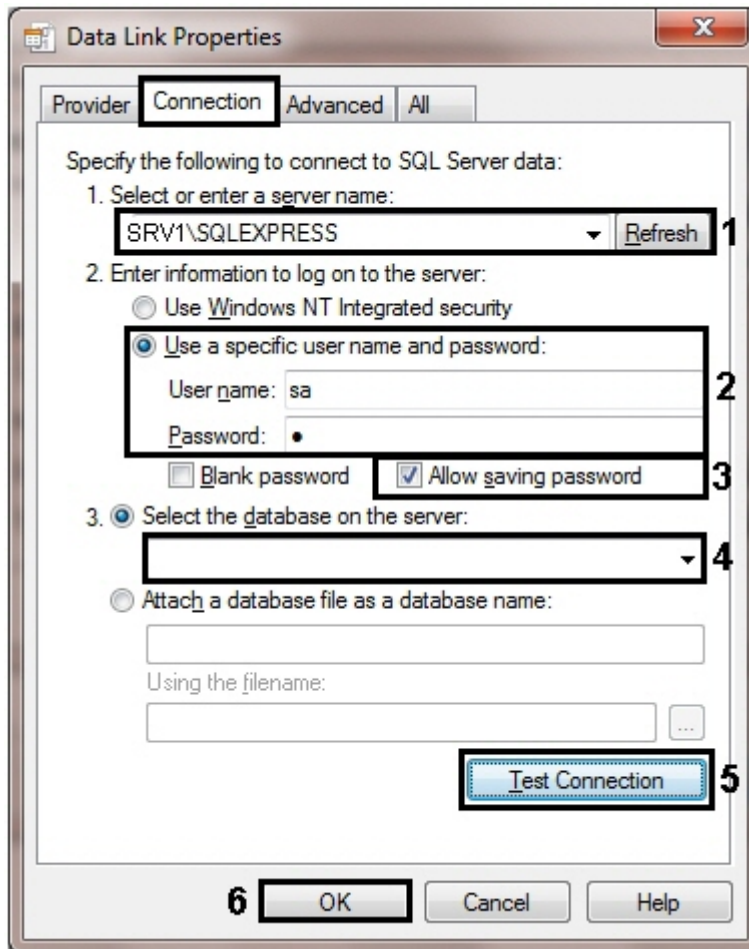


- c. In the **1. Select or enter a server name:** dropdown list select a name of DB server where the Server DB is stored (1).
- d. Set the **2. Enter information to log on to the sever:** to the **Use a specific user name and password:** position and specify the user name and password to connect to MS SQL Server (2).
- e. Select the **Allow saving password** check box (3).
- f. In the **Select the database on the server:** dropdown list select the name of the Server DB (4).
- g. Click the **Test Connection** button (5). If connection data is specified correctly, then the box with the **Test connection succeeded** message appears.

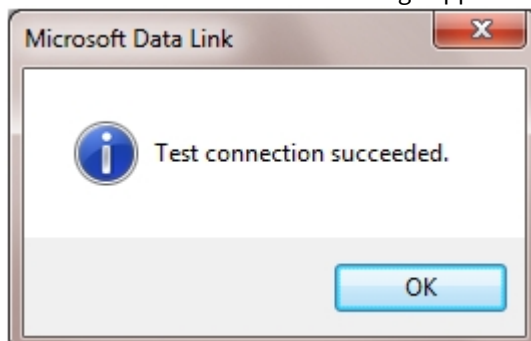


Note.

If there is the **Connection failed** message, then check if there is connection to the Server computer and if the server DB is configured correctly and then repeat steps 9.a-9.g.

- h. Click the **OK** button (6).
10. The configured connection string is displayed in the text field (8).
11. Click the **Main DB connection string** link (9). The **Data Link Properties** box appears. Configure DB connection to the base *Axxon PSIM* DB similarly to the Server (see steps 9.a-9.h). The configured connection string is displayed in the text field.
12. Click the  button to save the changes (10).

Note.


To remove the Server from the list, select it and click the  button (11).



Server is now added to the list.

8.1.3 Selecting active Server of Control

Select an active Server used by the *Additional workplace/Additional workplace of CSC* as follows:

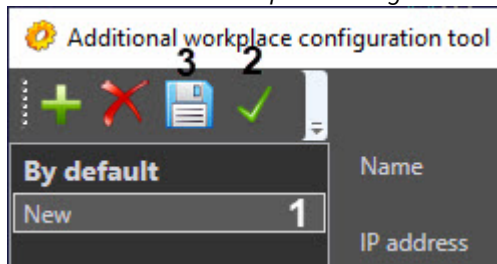1. Run the *Additional workplace configuration tool*.



2. Select the required Server in the list (1).
3. Click the  button (2).
4. Click the  button (3).

Active Server is now selected.

8.2 Working with Additional workplace/Additional workplace of CSC without Windows administration rights

To allow the user not added to the Administrators group in the Windows operating system to work correctly with *Additional workplace/Additional workplace of CSC*, make sure the user has the full access to the following registry section:

- for a 32-bit system: HKEY_LOCAL_MACHINE\Software\BitSoft\;
- for a 64-bit system: HKEY_LOCAL_MACHINE\Software\Wow6432Node\BitSoft\.

8.3 Creating and configuring Data Gateway


Data gateway is needed when live video is transmitted from *Agents of Control* to *Additional workplaces/Additional workplaces of CSC* in another subnet and *Monitoring PSIM* software components are not united in the distributed video surveillance system, as so as in this case **Video gate** object cannot be used.

The **Data Gateway** objects are created on the computers with *Server of Control/CSC* installed. The number of the **Data gateway** objects must be equal to the number of *Agent of Control* to receive live video from. For example, if there are 10 **Agents Of Control**, then create 10 **Data Gateways** with **Local port** and **Remote IP-address** corresponding to those *Agents of Control*.

In this section, the description of **Data Gateway** configuration is given. By default, this module is not enabled for live video transmitting to *Additional workplaces/Additional workplaces of CSC*. In order to enable Data gateway, set the **Viewing live video through gateway** in the **Monitoring** interface object settings panel – see [Configuring the Monitoring interface object](#).

Data Gateway object configuration is performed as follows:

1. Create the **Data Gateway** object based on the **Computer** object on the **Hardware** tab of the **System settings** dialog box.

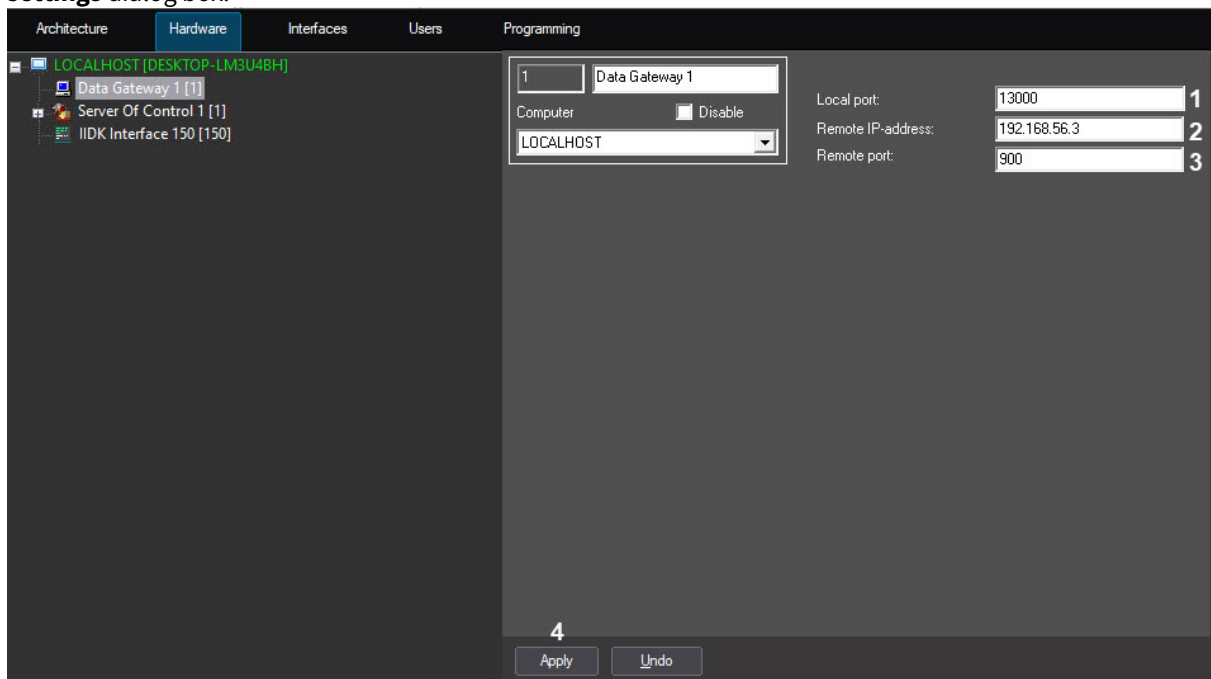

2. In the **Local port** field enter the number of the port in the system for connection of *Additional workplace/Additional workplace of CSC* (1).
3. In the **Remote IP-address** field enter IP-address of the *Agent of Control* (2).
4. In the **Remote port** field enter the standard port of the *Agent of Control* intended to transmit live video (3). Do not change the default value in most cases. It is to be changed only if by some reason the system uses intermediate server with port forwarding.
5. Click **Apply** (4).

Data Gateway configuration is completed.

9 Configuring the Monitoring PSIM fault tolerance

To configure the *Monitoring PSIM* fault tolerance, do the following:

1. Configure the main *Server of Control* (see [Configuring Server of Control](#)).
2. Configure the *Agent of Control* (see [Configuring Agent of Control](#)) and set the **Partition Of Control** connection to the main *Server of Control* (see [Configuring communication between Agent Of Control and Server Of Control](#)).
3. Create the second **Partition Of Control**, configure in the same way, but with a different **Partition Of Control** ID (see [Configuring the Partition Of Control unique ID](#)).
4. Configure a backup *Server of Control* (see [Configuring Server of Control](#)).
5. When configuring the second **Partition Of Control**, set the connection parameters to the backup *Server of Control* (see [Configuring communication between Agent Of Control and Server Of Control](#)).

 **Attention!**

If the list of cameras for tracking was added when configuring the first **Partition of Control** (see [Configuring the camera list](#)), then to add the same cameras to the second **Partition Of Control**, it is necessary to change the **MonitoringReserving** key value to **1** in the Windows registry (for details, see [Registry keys reference guide](#). for more information about working with the registry, see [Working with Windows OS registry](#)).

The *Monitoring PSIM* fault tolerance is configured.

10 Configuring the special mode of Monitoring operation with ACFA PSIM

On this page:

- [General information about special mode of Monitoring PSIM operation with ACFA PSIM](#)
- [Configuring the special mode of Monitoring PSIM operation with ACFA PSIM on the Server of Control side](#)
- [Configuring the special mode of Monitoring PSIM operation with ACFA PSIM on the Agent of Control side](#)
- [Operating procedure](#)

10.1 General information about special mode of *Monitoring PSIM* operation with *ACFA PSIM*


The special mode of *Monitoring PSIM* operation with *ACFA PSIM* allows to provide access to the object with the installed *Agent of Control* using the user's access card, and to monitor the object status on the *Server Of Control*. This operating mode is relevant if the *Monitoring PSIM* and *ACFA PSIM* are not combined into a single system with a distributed architecture.

10.2 Configuring the special mode of *Monitoring PSIM* operation with *ACFA PSIM* on the *Server of Control* side


The special mode of *Monitoring PSIM* operation with *ACFA PSIM* is configured on the *Server of Control* side as follows:

1. Create an **AccessByCardEnable** string registry key and set **1** as its value (for details, see [Registry keys reference guide](#), for more information about working with the registry, see [Working with Windows OS registry](#)).
2. Create the necessary number of access levels, which include one or more *Partitions of Control* of the corresponding *Agent of Control* objects, the access to which should be obtained. Do it as follows:

- a. In the **System Settings** dialog box, go to the **Programming** tab (1).

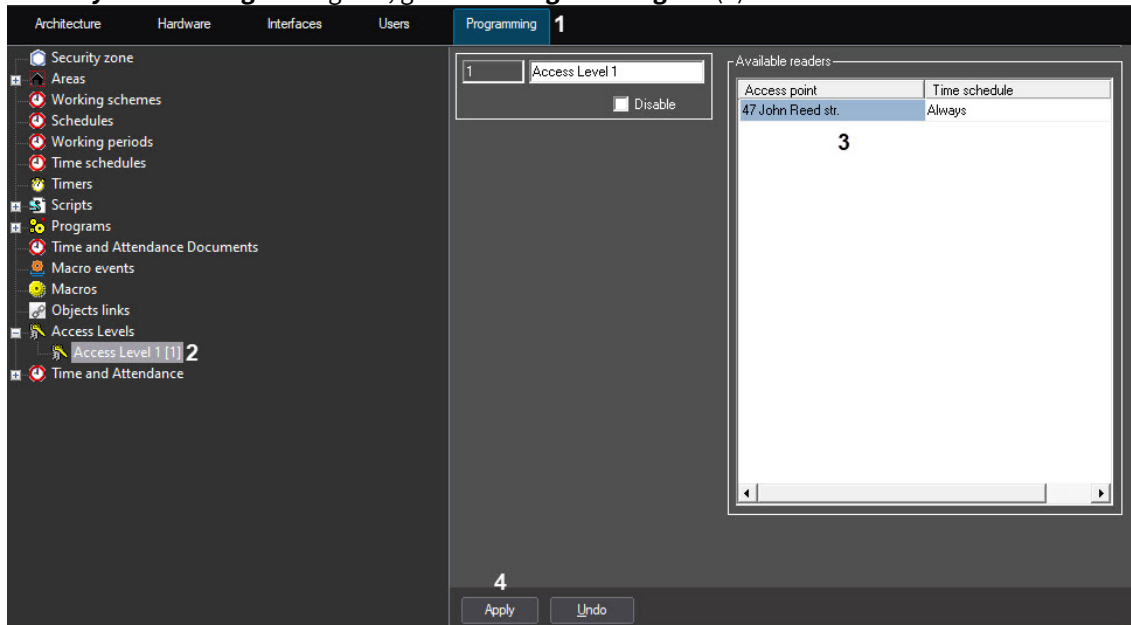

- b. In the object tree, create an **Access Level** object (2) on the basis of the **Access Levels** object.
 c. On the settings panel of this object, specify one or more access points to which the *Partitions of Control on Server of Control* correspond (3).
 d. Click **Apply** (4).
3. Create the necessary number of users who will be able to access objects, and assign an access card and access level to each user. Do it as follows:
- a. In the **System Settings** dialog box, go to the **Users** tab (1).

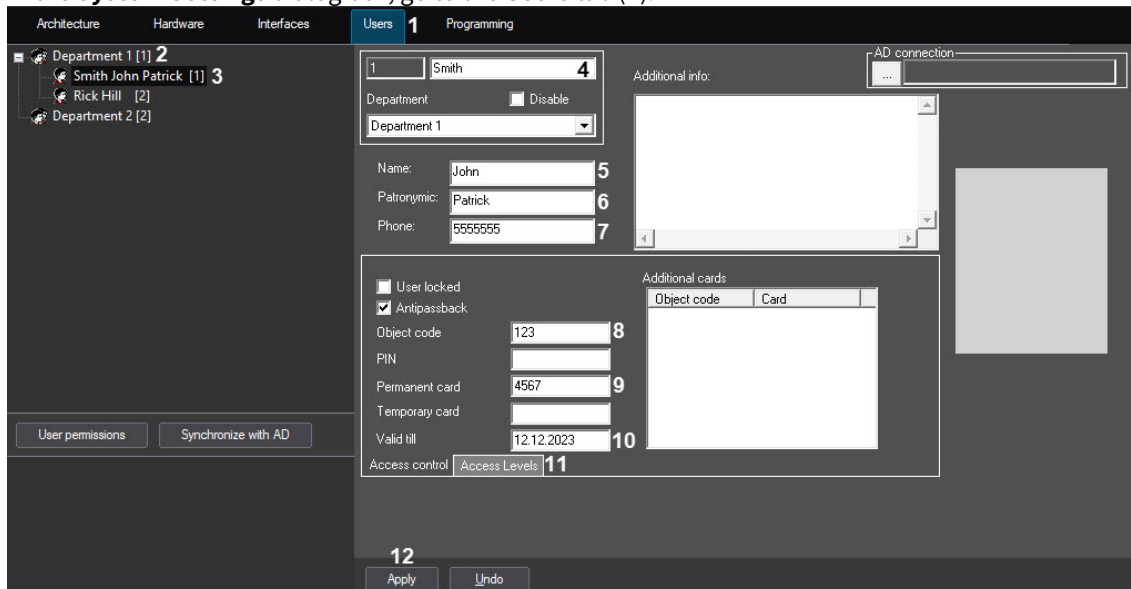

- b. In the object tree, create a **Department** object (2), and then create a **User** object (3) on its basis.
 c. On the settings panel of the **User** object, specify the following parameters:
- In the field (4) enter the last name of the user.
 - In the **Name** field (5), enter the first name of the user.
 - In the **Patronymic** field (6), enter the middle name of the user.
 - In the **Phone** field (7), enter the phone number of the user.
 - In the **Object code** field (8), enter the room code.

- f. In the **Permanent card** field (9) enter the card number.

Attention!

Both **Object code** and **Permanent card** fields should be filled in.

- g. If necessary, in the **Valid till** field (10), specify the date upon which access to the object will be restricted.
- h. Go to the **Access Levels** tab (11) and assign a previously created access level to the user (see step 2).

Access type:

A.L.	Date1	Time1	Date2	Time2
Access Level 1				

Access control | Access Levels

Apply Undo

- i. Click **Apply** (12).

Note

Similar actions can also be performed using the *Access Manager* module, which is part of the *ACFA PSIM* software package (see [Working with the Access Manager software module](#)).

Configuring the special mode of *Monitoring PSIM* operation with *ACFA PSIM* on the *Server of Control* side is complete.

10.3 Configuring the special mode of *Monitoring PSIM* operation with *ACFA PSIM* on the *Agent of Control* side


The special mode of *Monitoring PSIM* operation with *ACFA PSIM* is configured on the *Agent of Control* side as follows:

1. Create an **AccessByCardEnable** string registry key and set **1** as its value (for details, see [Registry keys reference guide](#), for more information about working with the registry, see [Working with Windows OS registry](#)).
2. Install *ACFA PSIM* (see [ACFA PSIM Installation Guide](#)).

Attention!

The following is an example of configuring the interaction between the *Monitoring PSIM* and the *Apollo* integration module, which is part of the *ACFA PSIM* software package. The configuration guide for the *Apollo* integration module is available in the documentation for *ACFA PSIM*. Instead of the *Apollo* integration module, you can use any other integration module that supports user entry into the controller.

3. Configure the *Apollo* integration module.
4. In the **System Settings** dialog box, go to the **Programming** tab (1).

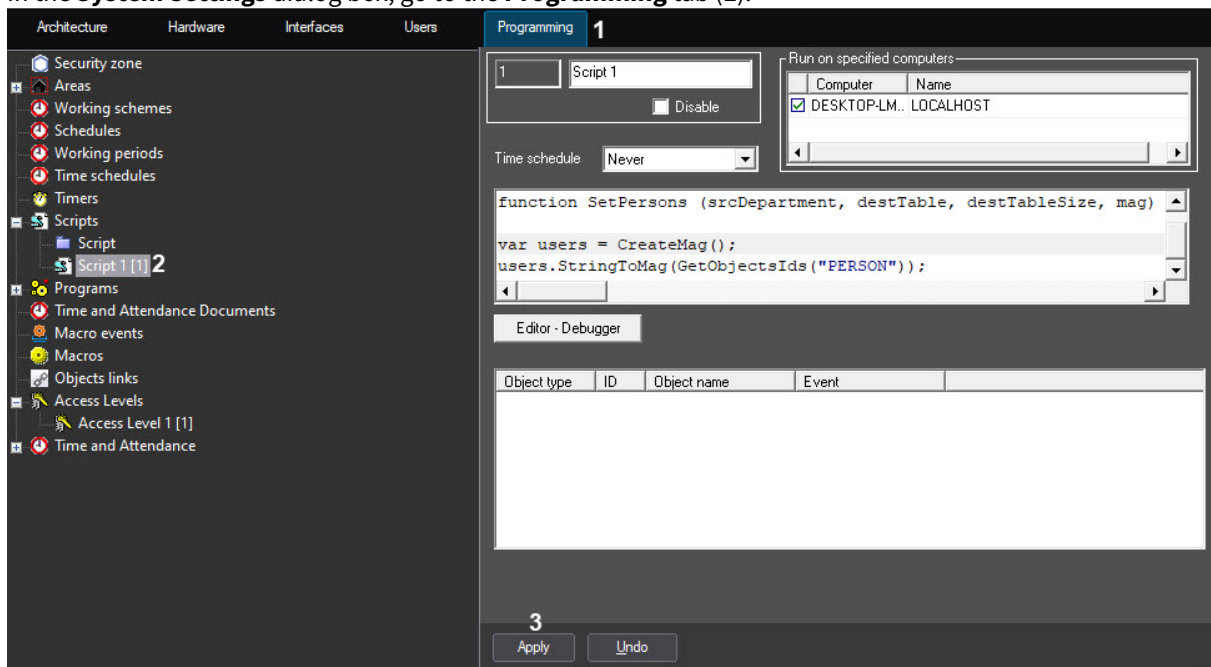

5. To transfer the user data from the *Server of Control* side to the *Agent of Control* side, it is necessary to create script №1 in the object tree on the basis of the **Scripts** object (2) by copying the contents of an example of this script (see [Sample script for configuring the interaction between the Monitoring PSIM and the Apollo integration module](#)).
6. To monitor the object status on the *Server Of Control* side, it is necessary to configure the alarm group (see [Configuring alarms for Monitoring PSIM the object state on the Agent of Control side](#)). As a result of this configuration, the script №2 will be created.

Attention!

If an integration module other than *Apollo* is used, it is necessary to modify the script examples for the corresponding integration module.

Note

For more information on creating scripts, see [The Script object. Programming using the JScript language](#).

7. Click **Apply** (3).

Configuring the special mode of *Monitoring PSIM* operation with *ACFA PSIM* on the *Agent of Control* side is complete.

10.4 Operating procedure


At startup, and then every 15 minutes, *Agent of Control* sends the hash of existing users to *Server of Control*. Initially, there are no such users. At startup, *Server of Control* receives the hash of all objects including users from the *Axxon PSIM* core, and puts them in a list that is updated if objects are edited or deleted. *Server of Control* compares the user hash received from *Agent of Control* with the value from the list and, if there is a mismatch, requests new data, and then transfers it to *Agent of Control*. *Agent of Control*, upon receiving this data (hash + configuration), updates the information about the users and generates the **SPR_DATA_UPDATED** event, which is processed in script №1. As a result, the users with the right to access the corresponding *Agent of Control* will be loaded into the memory of the *Apollo* controller and will be able to access the object upon presenting of their access card.

Also at startup, and then every 15 minutes, *Agent of Control* sends a **GET_OBJECT_STATE** event to the *Axxon PSIM* core. This event is processed in script №2, which generates an **OBJECT_STATE_INFO** event with the object status in the **state** field and the user's access card number used when arming/disarming the object in the **card** field. When arming an object using the user's access card, this script generates an **OBJ_ARM** event (alarm type: **Armed object**). When disarming an object using the user's access card, the same script generates the **OBJ_DISARM** event (alarm type: **Attention! Service personnel are working!**) and activates a long alarm **Object disarmed**.

Note

Only the user access card numbers are stored on the *Agent of Control* side, the users' full names are not available. Therefore, in order to obtain the users' full names by the access card numbers, *Server of Control* queries the *Axxon PSIM* database on the *Server of Control* side.

As a result, when the access to an object is received, the access card number and the full name of the user who gained the access is displayed in the **Event log** as an additional information (see [Event log](#)).

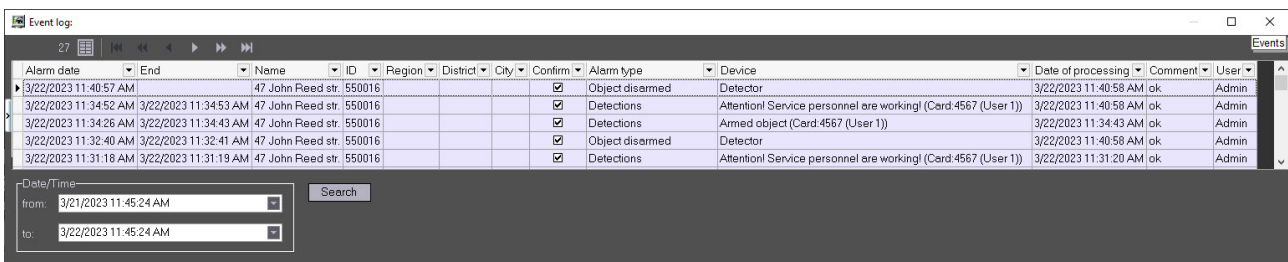


Alarm date	End	Name	ID	Region	District	City	Confirm	Alarm type	Device	Date of processing	Comment	User
3/22/2023 11:40:57 AM		47 John Reed str.	550016				<input checked="" type="checkbox"/>	Object disarmed	Detector	3/22/2023 11:40:58 AM	ok	Admin
3/22/2023 11:34:52 AM	3/22/2023 11:34:53 AM	47 John Reed str.	550016				<input checked="" type="checkbox"/>	Detections	Attention! Service personnel are working! (Card:4567 (User 1))	3/22/2023 11:40:58 AM	ok	Admin
3/22/2023 11:34:26 AM	3/22/2023 11:34:43 AM	47 John Reed str.	550016				<input checked="" type="checkbox"/>	Detections	Armed object (Card:4567 (User 1))	3/22/2023 11:34:43 AM	ok	Admin
3/22/2023 11:32:40 AM	3/22/2023 11:32:41 AM	47 John Reed str.	550016				<input checked="" type="checkbox"/>	Object disarmed	Detector	3/22/2023 11:40:58 AM	ok	Admin
3/22/2023 11:31:18 AM	3/22/2023 11:31:19 AM	47 John Reed str.	550016				<input checked="" type="checkbox"/>	Detections	Attention! Service personnel are working! (Card:4567 (User 1))	3/22/2023 11:31:20 AM	ok	Admin


11 Data loader for Monitoring

11.1 Server of Control communication module


Server of Control is a communication module that is responsible for receiving information from objects. The icon of the module (a red "V" symbol) is shown in the toolbar, in the lower-right corner of the screen.

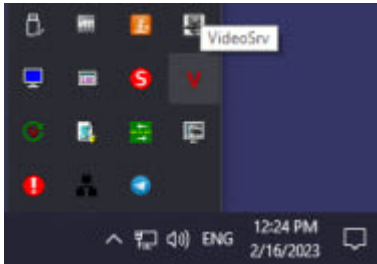

If you double click on the icon, the window shown in the following figure opens.

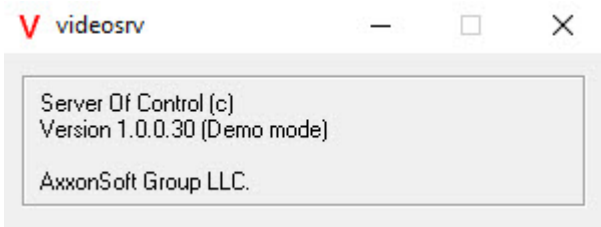


Server of Control starts automatically. If *Server of Control* has been stopped by mistake or any other reason, it can be restarted from **Start – All programs – Axxon PSIM – Monitoring PSIM – VideoSrv** menu.

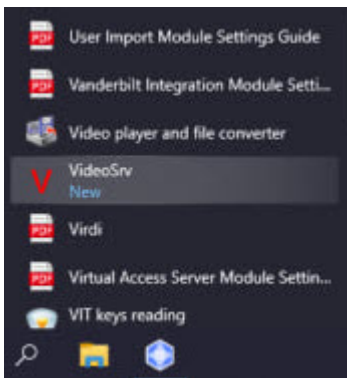


11.2 Data loader


Server of Control creates files that contain object status information and puts them in the exchange folder. The files are then loaded from the folder to the database by the *Data loader for Monitoring* module. The icon of the module (a "monitor" symbol) is shown in the toolbar, in the lower-right corner of the screen.

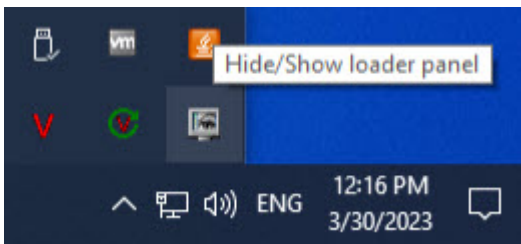

If you right-click on this icon, a context menu opens.

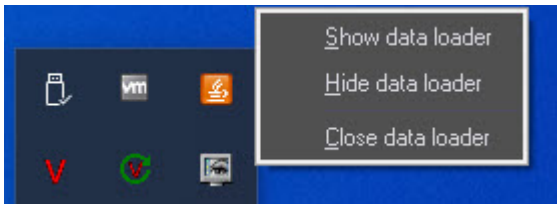

If you select the **Show data loader** menu item, the **Data loader for Monitoring** window opens.

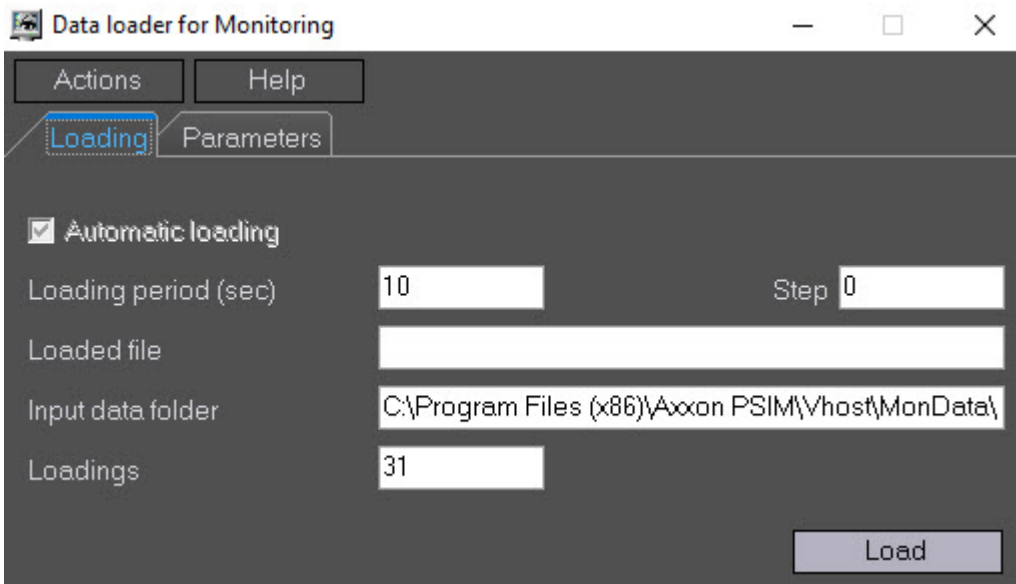


This window contains the following parameters:

1. **Input data folder:** the path to the folder that contains incoming files from *Server of Control*.
2. **Loading period (sec):** the time in seconds between two consecutive loads of incoming files from *Server of Control* into the database. This parameter applies to non-alarm messages. Alarm messages are recorded to the database immediately. Each time after data is loaded into the database, the system sends to the **Log panel** interface component a data update request. The **Log panel** refreshes the information from the database every minute.
3. **Automatic loading:** if you select this check box, data is loaded automatically. Otherwise, the load starts only when you click **Load**.
4. **Loaded file:** this field shows the name of the file being processed, or an error message if an error occurred while loading the data.
5. Message files received from *Server of Control* are processed in several steps. The current step is shown in the **Step** field.

11.3 Connecting to the database

To configure the database connection string, select the **Connection to database** item in the **Actions** menu.

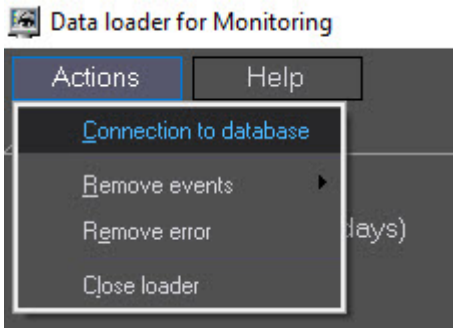


⚠ Attention!

If the location of the **MonitorSSTV** database changes from local to remote, then it is necessary to set the **0** value for the **UseBulkInsert** registry, if it changes from remote to local, then set the **1** value (for details, see [Registry keys reference guide](#). for more information about working with the registry, see [Working with Windows OS registry](#)).


11.4 Removing errors

If there was a failure while loading data, you cannot close the program in a usual way, because the loading process cannot be interrupted. To close the program, use the **Remove error** menu item.

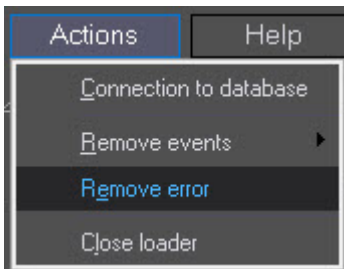

11.5 Removing events from the database

The **Remove events** menu item allows you to clear database. You can use the following modes:

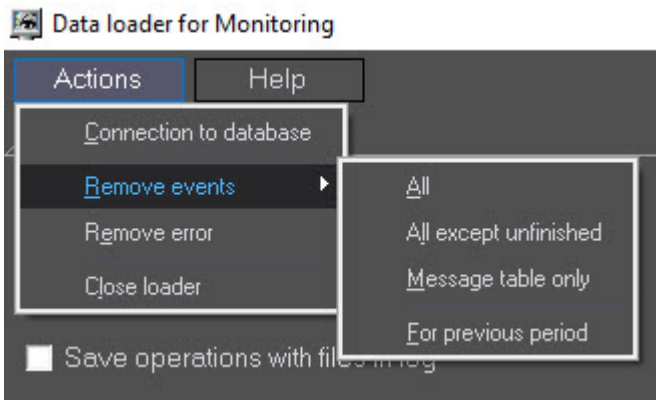


1. **All** – clears the database from alarms completely.
2. **All except unfinished** – clears the database from alarms completely, but leaves the information on the start of the alarm for those alarms that did not yet end (long-term alarms).
3. **Message table only** – clears the message log. This allows you to decrease the size of the database. In **Settings** tab, you can specify how long messages are kept in the log (see [Setting the log storage period](#)).
4. **For previous period** – clears the data for a specified period.

11.6 Setting the log storage period

If you want to specify how long the *Data loader* messages are kept in the log (event log), go to the **Data loader for Monitoring** window and then to the **Parameters** tab.

The data loader's event log is stored in the <Axxon PSIM software installation folder>\VHost\MONITOR\LOADER\LoaderSSTV_L_M.log, where M is a month.

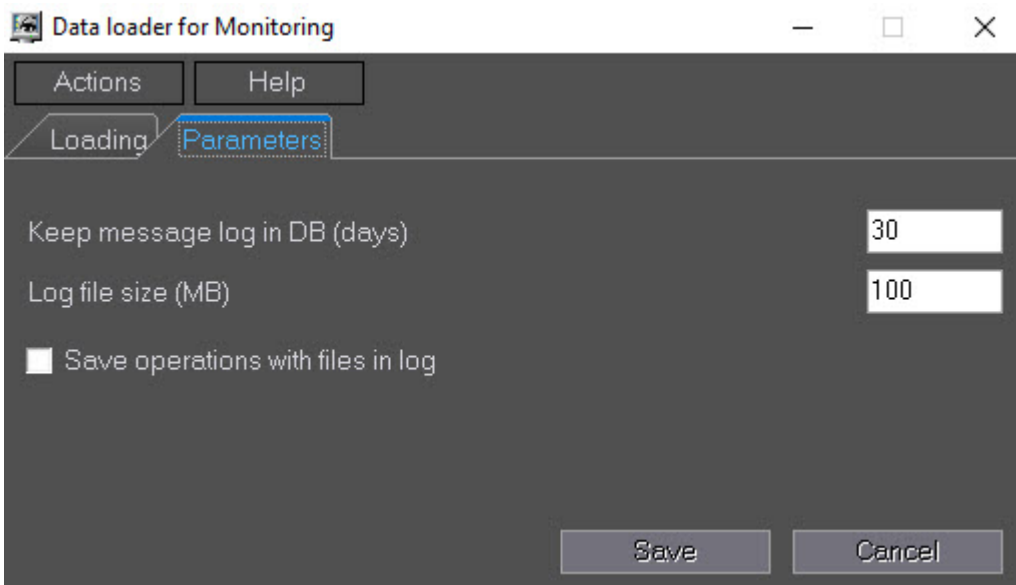

1. **Keep message log in DB (days)**: you can specify for how long will the data be kept in the **MonitorSSTV** database tables.
2. **Log file size (MB)**: you can specify the file size for the data loader's event log (in megabytes). After this limit is reached, the log file is archived.
3. **Save operations with files in log**: this allows you to save details for the data loader's file operations in the data loader's event log.

11.7 Configuring automated video clip loading

To enable automated video clip loading, set the **FileQueryEnable** key in the Windows registry to **1** and specify folder to share data with third party system in the **FileQueryPath** key (see [Registry keys reference guide](#) for more details on the key and the [Working with Windows OS registry](#) section of *Axxon PSIM software. Administrator's Guide* for more details on how to operate registry keys). Restart the computer to ensure the changes applied.



Note.

The **C:\Query** folder is set by **FileQueryPath** key by default.



Important!

Specify different folders in **FileQueryPath** key if automated video clip loading is enabled both on *Server of Control* and *Additional workplace* simultaneously.



Note.

When *videosrv.exe* communication module starts at the *Server of Control*, the folder specified in the **FileQueryPath** key is automatically created with the following subfolders:

In – the folder for request files;

In\Work – the service folder for request files;

OutSuccess – the folder to place request files in after successful load of the video clips;

OutError – the folder for incorrect request files or request files with absent mandatory parameters;

OutFail – the folder to place correct request files in if video clip could not be loaded for some reason.



Important!


At *Additional workplace*, create the folder specified in the **FileQueryPath** key with all subfolders described above manually.

11.8 Specifying the export directory

An export directory is automatically created on the *Server of Control* and on the *Central Server of Control* to save all requested frames and video fragments. By default, the export directory is located at **DISK:\Export**, where **DISK** is the drive on which the operating system is installed. You can change the path to this directory using the **ExportPath** registry key (see [Registry keys reference guide](#)). Then the *Monitoring reports* and *Search in archive* modules can work with this data storage.

If necessary, you can configure saving frames and video fragments in the *Monitoring PSIM* database on the *Server of Control* (**MonitorSSTV**) and the *Central Server of Control* (**ServerSSTV**) instead of the export directory. For this purpose, it is necessary to set the string parameter of the **KeepVideoDataInBase** registry key equal to the number of days of storage in the database (see [Vertical solutions](#)). The data is stored in the *video_data* table.

To restore data from the *Monitoring PSIM* database to the export directory, use the *RestoreExportDir.exe* utility that is installed on the *Server of Control* and on the *Central Server of Control* at the *<Axxon PSIM installation directory>\Vhost\SYSTEM* path. To start restoring data, click the **Restore export folder** button.

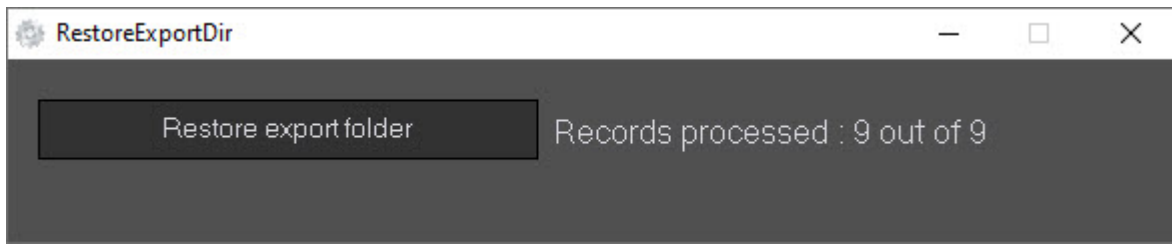


12 Configuration of the Monitoring PSIM interface

12.1 General information about the Monitoring PSIM interface

The *Monitoring PSIM* interface is accessible through the following interface elements

1. **Monitoring.**
2. **Monitoring reports.**
3. **Search in archive.**

These objects are created based on the **Display** object, in the **Interfaces** tab of the **System settings** dialog box. It is recommended to create these objects on the basis of different **Display** objects.

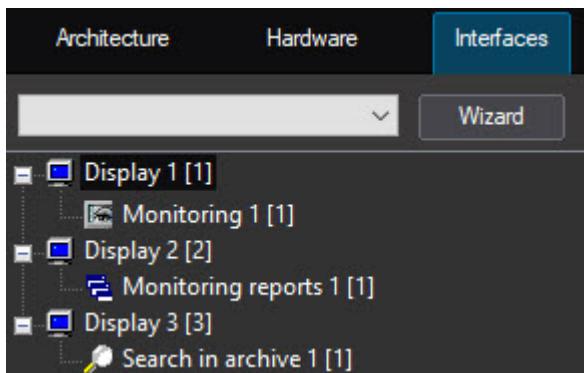

Interface objects are available at the following *Monitoring PSIM* installation types: *Server of control*, *Additional workplace*.

Note.

Operations with interface objects are described in the [Monitoring PSIM. Operator's Guide](#) document.

12.2 Configuring the Monitoring interface object

Attention!

Before creating the **Monitoring** object, create and configure the **Server Of Control** object (see [Creating necessary Server Of Control objects](#)).

To configure the **Monitoring** interface object:

1. In the object tree, select the **Monitoring** object. On the right side of the **System settings** dialog box, the settings panel of the relevant object is displayed.



2. Set the checkboxes next to the alarm groups that should be visualized (1). The **Extra 1** and **Extra 2** groups of alarms can be renamed (2).
3. If it is necessary to display the **Owners panel** component on the screen, set the **Owners panel** checkbox and specify the component position coordinates on the monitor screen. Also, from the **Monitor** drop-down list, select the number of the physical monitor, which coordinates should be specified (3). You can also set the scaling of objects from 100% to 500%.

Note

If the scaling parameter exceeds 110%, then the high resolution icons will be displayed on the object, and the Courier New font will be used for the text in the object title, otherwise—MS Sans Serif.

4. If it is necessary to display the **Control panel** component on the screen, set the **Control panel** checkbox and specify the component position coordinates on the monitor screen. Also, from the **Monitor** drop-down list, select the number of the physical monitor, which coordinates should be specified (4). You can also set the scaling of objects from 100% to 500%.

Note

If the scaling parameter exceeds 110%, then the high resolution icons will be displayed on the object, and the Courier New font will be used for the text in the object title, otherwise—MS Sans Serif.

5. If it is necessary to display the **Log panel** component on the screen, set the **Log panel** checkbox and specify the component position coordinates on the monitor screen. Also, from the **Monitor** drop-down list, select the number of the physical monitor, which coordinates should be specified (5).
6. Set the **Non-empty Comment field** checkbox, if it is necessary for the operator to comment on this alarm and/or their actions, when accepting the alarm (6). This comment can be viewed later in the event log, as well as the name of the operator who received the alarm.
7. By default, objects can be filtered by **Alarm** and **Failure** events as well as by **Connected** and **Disconnected** states. Clear the **Use filter by events** checkbox to disable this feature (7). As a result, the corresponding drop-down list becomes disabled.
8. When you try to view live video and want to display a warning that it can create the critical load on the channel, set the **Warning when watching live video** checkbox (8).
9. If *Agents Of Control* and *Additional workplaces* are in different subnets and the *Monitoring PSIM* components are not in a distributed system configuration in *Axxon PSIM* object tree and **Data gateway** is in use for transmission of live video to *Additional workplaces*, set the **Viewing live video through gateway** checkbox (9).

 **Note**

For the details about the **Data gateway**, see [Creating and configuring Data Gateway](#).

10. To add the **All cameras of Partition Of Control** item to the object's **Video image playback** context menu which enables viewing video from all cameras of the selected *Partition Of Control*, set the **Viewing live video from all cameras (add.)** checkbox (10).
11. In the **Video stream speed** field, enter the number of frames per second of the video image when viewing live or archive video (11). This parameter is used to limit the data flow between the *Server Of Control* and the *Agent Of Control* (for example, in case the communication channel has low bandwidth).

 **Note**

- If the archive is recorded with the H.264 codec and the video stream speed is set to more than **0** frames per second, then the archive video will be played back only by reference frames.
- If the value of the video stream speed is **0**, then the live and archive video will be played back without scaling.

12. Select the required compression rate for the live video from the **Compression** drop-down list (12).
13. If it is necessary to set the cameras for which the user should be prohibited from viewing live video, do the following:
 - a. Click the **Cameras** button (13).

b. The settings window will open:





- c. In the **User** drop-down list (1), select the user to whom the prohibition should be applied.
- d. The **List of cameras prohibited for viewing** field (2) displays the cameras prohibited from viewing for the selected user. To add a camera to the list, select the required object from the **Object** drop-down list (3) and click the button.

Note


The **Object** list contains only those objects that have cameras.

- e. A window with a list of cameras of this object will open:

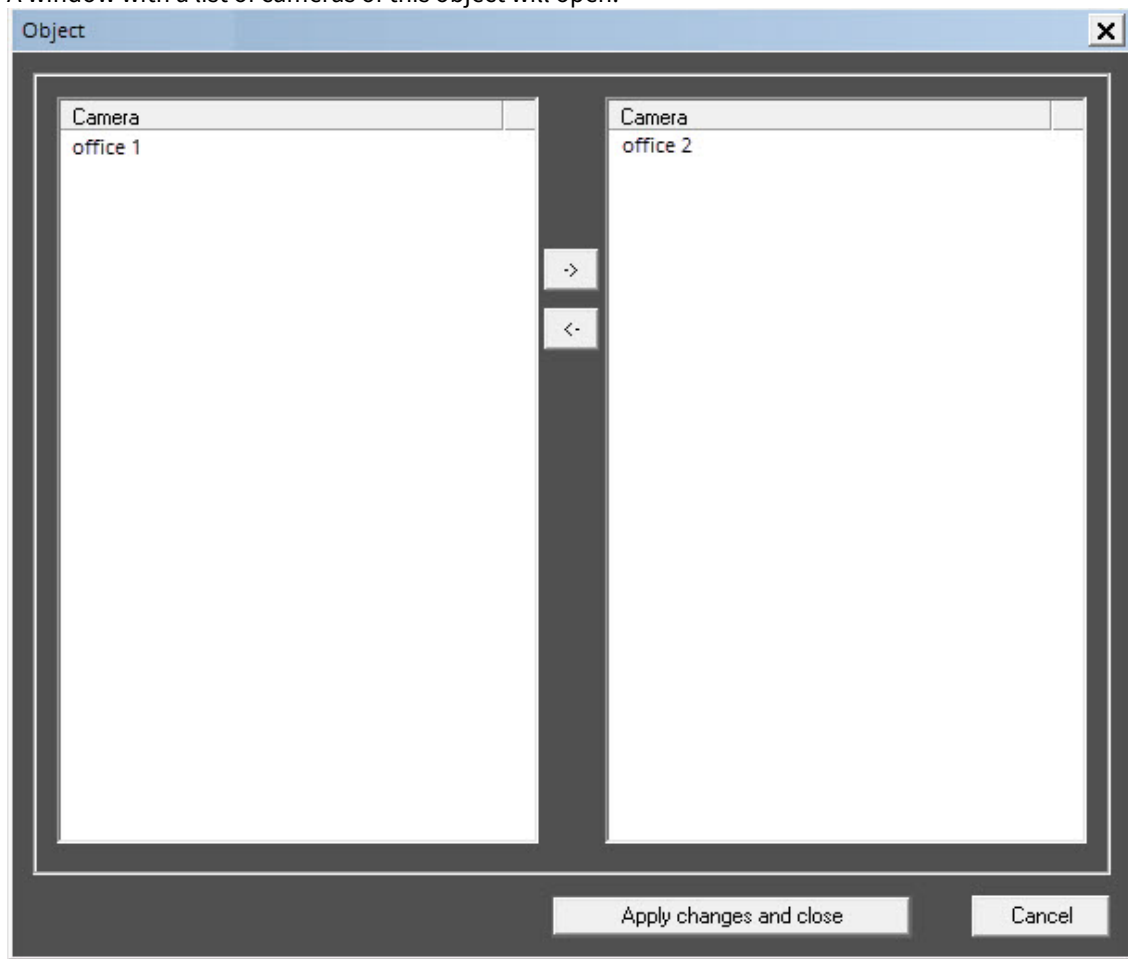

- f. In the left part of the window, select the cameras that should be prohibited from viewing, and move them to the right part of the window using the  button. Then click the **Apply changes and close** button.

Note

To cancel the prohibition, select the camera in the right part of the window and click the  button.


- g. Click the **OK** button (4).

Note

- If a filter by owner is used for the **Monitoring** interface object, then its value is taken into account when configuring prohibited cameras.
- If the user selects a camera that is not prohibited from viewing live video in the **Monitoring** interface, they can enter the camera's function menu and select a camera prohibited from viewing using the Camera menu item. To prevent this from happening, it is necessary to hide the Camera menu item using the MENU_CAMS_DISABLE_OPTION registry key (see [Registry keys reference guide](#)).



- When adding a camera to the list of prohibited from viewing, the camera is not automatically removed from the previously created screens to which this camera was added.

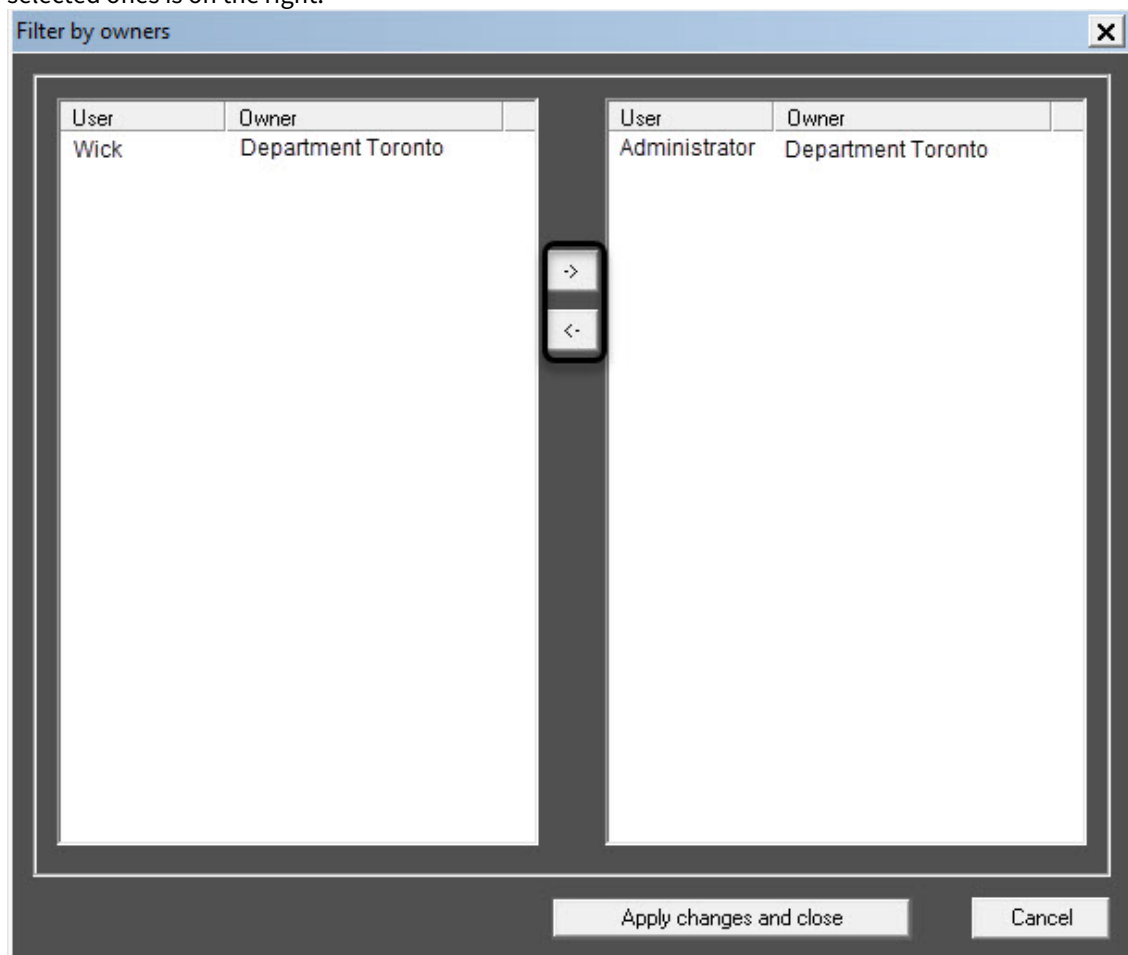14. If specific owners are to be available for specific users on the **Owners panel**, then set the filter by owners:
 - a. Click the **Filter** button (15).
 - b. The **Filter by owners** window appears. The list of available user-owner pairs is on the left, the list of selected ones is on the right.



Note

The list of owners is set on the **Control panel**—see [Regulatory and reference information](#). Users and their rights are configured in the **Users** tab of the **System settings** dialog box—for details, see [Limiting access to the system objects administration, control and viewing functions](#).

- c. Move the pairs between the lists using the  and  buttons.
 - d. When the list of user-owner pairs is formed, click the **Apply changes and close** button.
15. Selected pairs of users and owners are displayed in the table (14).
 16. Click the **Apply** button (16).

Configuration of the **Monitoring** interface object is now complete.

When a screen for which the **Monitoring** object has been created is selected in *Axxon PSIM*, the **Monitoring** interface window is displayed.

12.3 Configuring the Search in archive object

The **Search in archive** interface object is configured as follows:

1. Select the **Search in archive** object in the objects tree. In the right part of the **System settings** dialog box, the settings panel for this object will be displayed:

2. From the **Monitor** drop-down list, select the number of the physical monitor, which coordinates should be specified. Specify the **Search in archive** window position coordinates on the screen of the selected monitor (1).
3. Set up a filter by owners (2) by analogy with the **Monitoring** interface object—see [Configuring the Monitoring interface object](#).
4. Click the **Apply** button (3).

When you select the **Display** object on the basis of which the **Search in archive** object was created in *Axxon PSIM*, the **Search in archive** interface window will be visualized (see [Search in archive](#)).

12.4 Configuration of the Monitoring reports object

To configure the **Monitoring reports** object, do the following:

1. Select the **Monitoring reports** object in the objects tree. The settings panel of the object is displayed to the right of the **System settings** dialog box.

The screenshot shows the 'Monitoring reports' settings panel. At the top left, there is a text input field containing '1' and a label 'Monitoring reports 1'. Below it is a 'Display' section with a dropdown menu showing 'Display 2'. To the right is the 'Position' section with input fields for X (0), Y (0), W (100), and H (100), and a 'Monitor' dropdown menu set to '1'. Below the position section is a 'Filter by owners' table with columns 'User' and 'Owner', and a large empty space labeled '2'. To the right of the table is a 'Filter ...' button. On the far right is the 'Reports' section with checkboxes for 'System failures', 'Alarms', 'Video report', 'Operator actions', 'Statistics', 'Statistics by owners', and 'Vehicle LPs'. Under 'Vehicle LPs' are two radio buttons: 'Full access' (selected) and 'Marketing'. At the bottom of the panel are 'Apply' and 'Undo' buttons, with the number '5' above the 'Apply' button.

2. From the **Monitor** drop-down list, select the number of the physical monitor, which coordinates should be specified. Specify the **Monitoring reports** window position coordinates on the screen of the selected monitor (1).
3. Set the filter by owners similar to the one for the **Monitoring** object (2), see [Configuring the Monitoring interface object](#).
4. By default, all reports are available for the operator. To hide some of the reports, clear the checkboxes next to them in the **Reports** group (3).
5. Select the type of access to the Vehicle LPs reports (4):
 - a. **Full access**: all Vehicle LPs report types are available.
 - b. **Marketing**: only the average time span at the gas station and number of vehicles reports are available, and the Vehicle LP field is restricted to three letters and a % character.
6. Click the **Apply** button (5).

Configuration of the **Monitoring reports** object is completed.

13 Configuring audio calls from the Monitoring interface

13.1 General information

Audio calls are supported between operators in a distributed configuration on the *Server Of Control/Agent Of Control* side. Audio calls are made using the **SIP-terminal** object. Physical SIP devices are not required.

13.2 Configuring audio calls from the Monitoring interface


Configure audio calls from the **Monitoring** interface as follows:

1. At the *Server Of Control* and *Agent Of Control* side:
 - a. Create the **Audio card** object with the **Microphone** child object (see [Audio subsystem configuration](#)).
 - b. Create the **Audio playback card** object with the **Speaker** child object (see [Configuring audio playback](#)).
2. At the *Server Of Control* side:
 - a. Create the **SIP-terminal** object as a SIP-server in *Axxon PSIM* (see [Configuring SIP-terminal](#)).
 - b. On the basis of the **SIP-terminal** object, create two **SIP-operator** child objects and for each of them specify the corresponding operator identification number ([Configuring SIP-operators of the Axxon PSIM's SIP server](#)).
 - c. On the basis of the **SIP-terminal** object, create the **Address book** object and select the previously created SIP-operators (see [Configuring address book of SIP-terminal](#)).
 - d. On the settings panel of each **SIP-operator**, select a previously created address book (see [Configuring SIP-operators of the Axxon PSIM's SIP server](#)).
 - e. Create the **SIP-panel 1** interface object on the same **Display 1** object on which the **Monitoring** interface object was created (see [Configuring the SIP-panel interface object](#)).


Note

Recommended coordinates of the SIP-panel: X = 40, Y = 40, W = 20, H = 21.


- i. On the **Basic settings** tab of the **SIP-panel 1** object, select the **SIP-terminal** as the terminal (see [Basic settings of the SIP-panel interface object](#)).
- ii. On the **Advanced settings** tab of the **SIP-panel 1** object, set the checkboxes as shown in the figure below (see [Advanced settings of the SIP-panel interface object](#)).

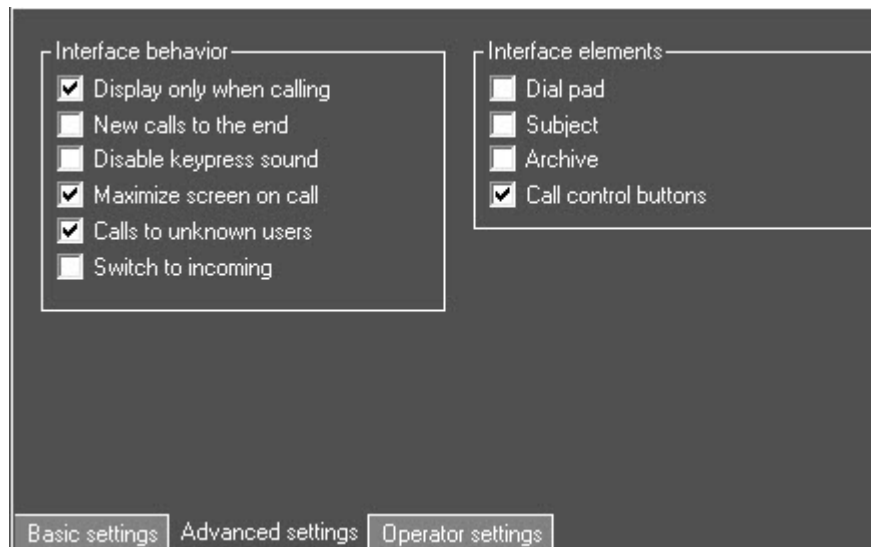


- iii. On the **Operator settings** tab of the **SIP-panel 1** object, configure the list of SIP-operators as shown in the figure below (see [Operator settings of the SIP-panel interface object](#)).

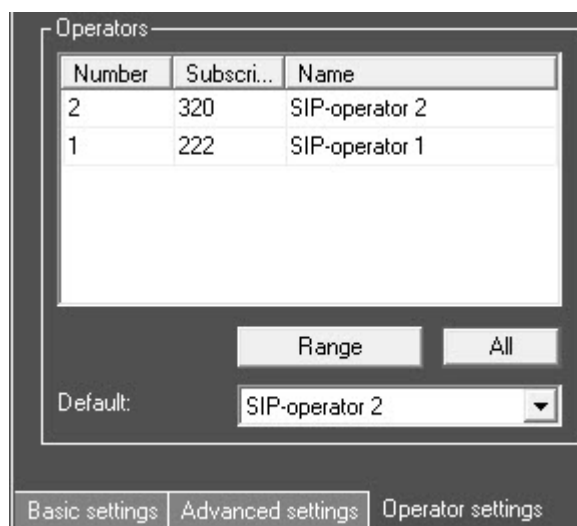

- f. Create the **Display 2** object, which will be displayed only on the *Agent Of Control* side (see [Assigning the displays to the operator workstations](#)).
- g. Create the **SIP-panel 2** child interface object.
- i. On the **Basic settings** tab of the **SIP-panel 2** object, select the **SIP-terminal** as the terminal (see [Basic settings of the SIP-panel interface object](#)).
 - ii. On the **Advanced settings** tab of the **SIP-panel 2** object, set the checkboxes as shown in the figure below (see [Advanced settings of the SIP-panel interface object](#)).

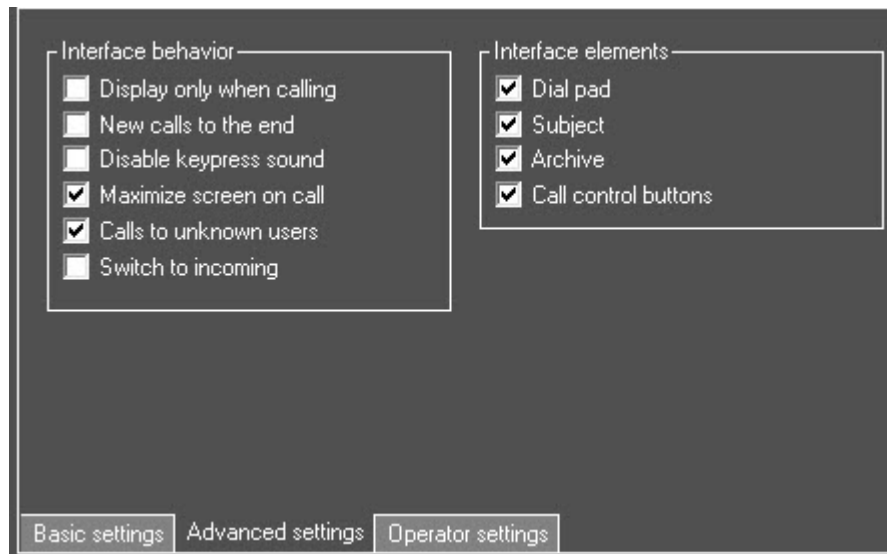


- iii. On the **Operator settings** tab of the **SIP-panel 2** object, configure the list of SIP-operators as shown in the figure below (see [Operator settings of the SIP-panel interface object](#)).

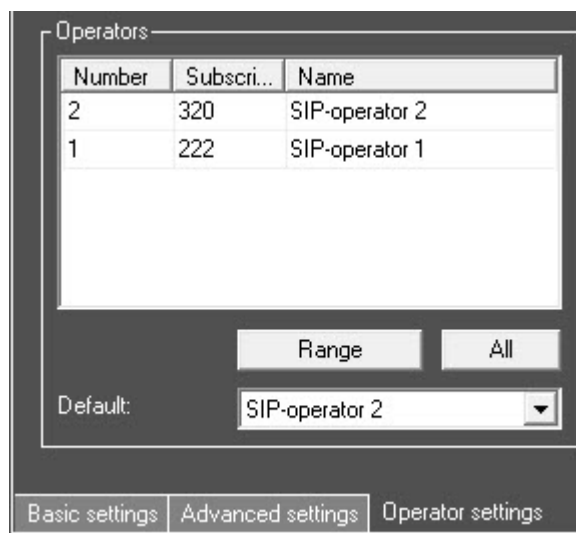

- h. On the settings panel of the **Computer** object, select the speaker and microphone of the SIP-operator (see [Selecting speaker, microphone and camera for SIP-operator](#)).

Configuring audio calls from the **Monitoring** interface is now complete.

As a result, the **Audio call** item will appear in the context menu of the object in the **Monitoring** interface. When you select this menu item, an audio call will be made to the operator who is on the computer with the corresponding object.

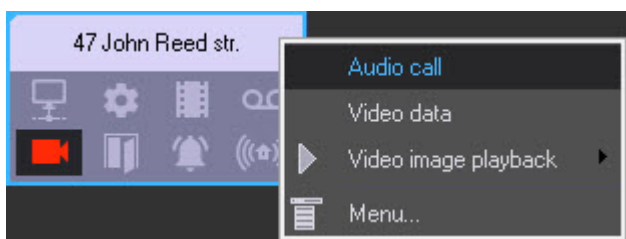


14 Configuring special operation mode joint with Auto PSIM


14.1 Configuration on the Agent Of Control side

Configure special operation mode on *Agent Of Control* as follows:


1. Create and configure the **Agent Of Control** object on the **Hardware** tab (see [Configuring Agent of Control](#)).
2. Create and configure the **LPR channel** object on the **Hardware** tab (see [Auto PSIM Guide](#)).

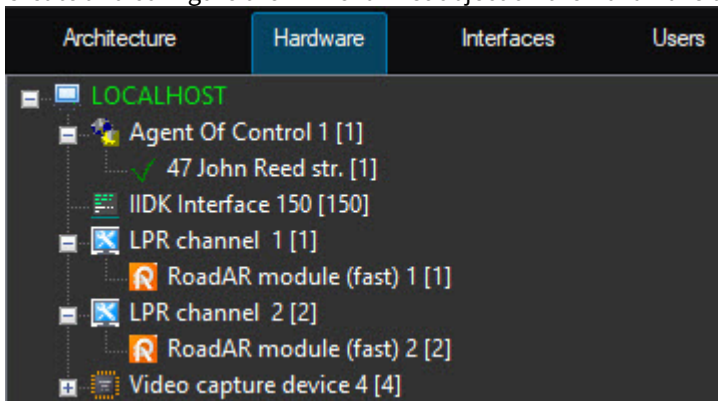

3. Create the **Partition Of Control** object on the basis of the **Agent Of Control** object, then add to it the **LP recognized** events for entrance and exit (see [Configuring the Partition Of Control object](#)).

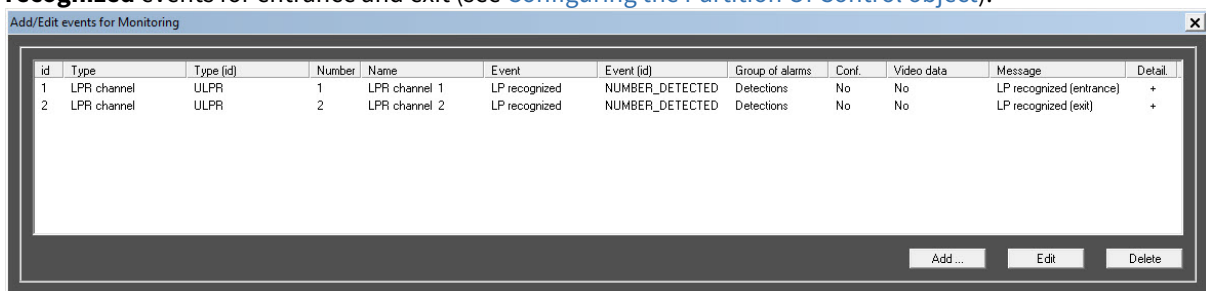

4. Create the **ULPR** section in the Windows registry if it is not created yet (see [Registry keys reference guide](#). For more details on how to operate the registry, see [Working with Windows OS registry](#)).
5. In the **ULPR** section of the Windows registry, create the **ULPRspecialProcessing** string parameter and set its value to **1** (see [Registry keys reference guide](#). For more details on how to operate the registry, see [Working with Windows OS registry](#)).
6. In the **ULPR** section of the Windows registry create the **PlaceOfRecognitionN** string parameter, where **N** is the ID of the **LPR channel** object.
This parameter corresponds to the point of recognition. Value **1** corresponds to entrance. Value **2** corresponds to exit (see [Registry keys reference guide](#). For more details on how to operate the registry, see [Working with Windows OS registry](#)).

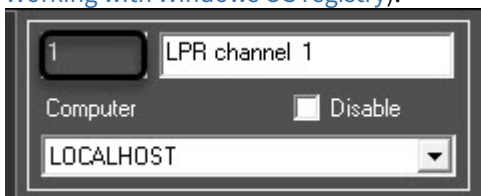

7. In the **ULPR** section of the Windows registry (see step 4) create the **CamOfRecognitionN** string parameter, where **N** is the ID of the **LPR channel** object. The value in this key should correspond to the ID of the **Camera** object specified in the **LPR channel** object settings (see [Registry keys reference guide](#). For more details on

how to operate the registry, see [Working with Windows OS registry](#)).




- Restart the computer to apply the changes.

Configuring the special operation mode on the *Agent Of Control* side is now completed.

14.2 Configuration on the Server Of Control side

Configure the special operation mode on the *Server Of Control* side as follows:

- Create and configure the **Server Of Control** object on the **Hardware** tab (see [Configuring Server of Control](#)).
- Create and configure one or several **External Plates DB** objects on the **Hardware** tab (see [Connecting and setting up of the external LP number database](#)).
- Create and configure the **Monitoring** object on the **Interfaces** tab (see [Configuring the Monitoring interface object](#)).

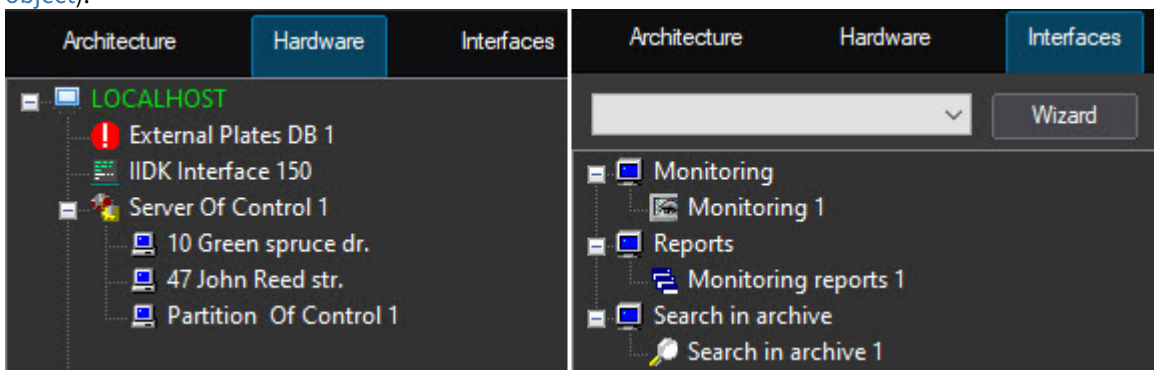

- Create the **ULPR** section in the Windows registry if it is not created yet (see [Registry keys reference guide](#). For more details on how to operate the registry, see [Working with Windows OS registry](#)).
- In the **ULPR** section of the Windows registry, create the **ULPRspecialProcessing** string parameter and set its value to **1** (see [Registry keys reference guide](#). For more details on how to operate the registry, see [Working with Windows OS registry](#)).
- Restart the computer to apply the changes.

As a result, the **Info on vehicle license plates** button becomes available in the **Log panel** and **Details** window of the **Monitoring** interface. The **License plate search** window opens when you click this button (see [Viewing recognized LPs](#)).

ID	Name	Cameras	Disk_GB	Info on vehicle license plates	First record	Disks temp.	Memory_MB	Work duration	Software version	2:15 PM	2:30 PM	2:45 PM	3:00 PM	3:15 PM
550016	47 John Reed str.	4	474	1 192.168.1.2	2/10/2023	35 °C	11359	0 01:01	1.0.56	-	-	-	-	-
550017	10 Green spruce dr.	1	474	1 192.168.1.2	3/16/2023	35 °C	11359	0 01:01	1.0.56	-	-	-	-	-
550018	Partition Of Control 1													

Object code	ID	Name	Cameras	Disk_GB	Disks	Info on vehicle license plates	brd	Disks temp.	CPU usage, %	Memory_MB	Total memory_MB	Work duration	Software version	Core version
1	550016	47 John Reed str.	4	474	1	192.168.1.2	2/10/2023	35 °C	18	11359	16328	0 01:01	1.0.56	1.0.0.488
2	550017	10 Green spruce dr.	1	474	1	192.168.1.2	3/16/2023	35 °C	18	11359	16328	0 01:01	1.0.56	1.0.0.488
3	550018	Partition Of Control 1												

 **Note**


By default, the **LP found in the database** alarm is generated for the **Entrance** recognition point only. In order to generate alarm both on **Entrance** and **Exit** points, in the **ULPR** section of the Windows registry, create the **AlarmMsgOne** string parameter and set its value to **0** (see [Registry keys reference guide](#). For more details on how to operate the registry, see [Working with Windows OS registry](#)).

Configuring the special operation mode on the *Server Of Control* side is now completed.

15 Appendix 1. Interfaces

15.1 Settings panel of the Agent Of Control object

Settings panel of the **Agent Of Control** object is given on figure.

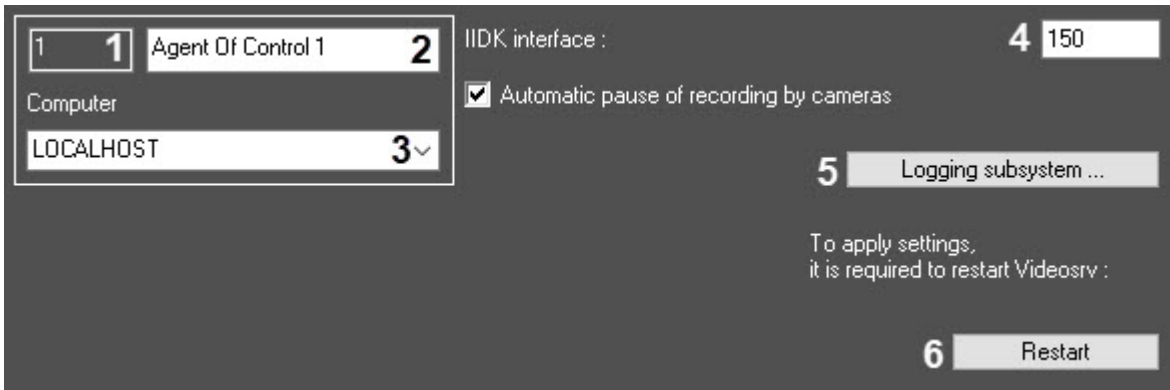

Description of the **Agent Of Control** object settings panel elements is given in table.

#	Parameter	Method for setting the parameter value	Description	Type	Default value	Value range
1	Identifier	Automatically	Shows the identification number of the Agent Of Control object in the system	Nonnegative integer	-	≥ 0
2	Name	Enter the value in the field	Shows the name of the Agent Of Control object in the system	Latin letters and service characters	Agent Of Control	A line representing a sequence of any symbols (letters, digits, service characters apart from > and < symbols), not case-sensitive. Number of symbols – from 1 to 60
3	Computer	Is selected in the list	Assigns the parent Computer object for the Agent Of Control object	Name of the Computer objects registered in the system	Name of the parent Computer object	Depends on the number of the Computer objects in the system

#	Parameter	Method for setting the parameter value	Description	Type	Default value	Value range
4	IIDK interface	Enter the value in the field	Sets the ID number of IIDK interface object used by the Agent Of Control object	Nonnegative integer	150	≥ 0
5	Logging subsystem ...	Click the button	Opens a dialog box for setting logging subsystem parameters	-	-	-
6	Restart	Click the button	VideoSrv communication module restarting	-	-	-

15.2 Settings panel of the Partition Of Control object

Settings panel of the **Partition Of Control** object is given on figure.

The screenshot shows the configuration interface for a 'Partition Of Control' object. It includes the following elements:

- 1**: Identifier field containing '1'.
- 2**: Name field containing 'Partition Of Control 1'.
- 3**: Agent Of Control dropdown menu showing 'Agent Of Control 1'.
- 4**: ID field containing '386'.
- 5**: TCP port (UPS) field containing '8888'.
- 6**: Transmitting ... button.
- 7**: Monitoring ... button.
- 8**: Video data ... button.
- 9**: Cameras table with one entry:

Number	Keep archive for (days)
1	60/0
- 10**: Cameras ... button.
- 11**: Sensors table with one entry:

Sensor ID	Sensor type
1	Vibration sensor (frames,captions)
- 12**: Add ... button.
- 13**: Edit ... button.
- 14**: Delete button.
- Registration status: No connection.
- Total cameras: 1.
- Sensors: 1.
- Apply and Undo buttons at the bottom.

Description of the **Partition Of Control** object settings panel elements is given in table.

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
1	Identifier	Enter the value in the field	Shows the identification number of the Partition Of Control object in the system	Latin letters and service characters	-	-

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
2	Name	Enter the value in the field	Shows the name of the Partition Of Control object in the system	Latin letters and service characters	Partition Of Control	A line representing a sequence of any symbols (letters, digits, service characters excluding characters: underscore "_", backslash "\", angle brackets ">" and "<", single quote "'"). Number of symbols – from 1 to 60
3	Agent Of Control	Is selected in the list	Assigns the parent Agent Of Control object for the Partition Of Control object	Names of Agent Of Control objects registered in the system	Name of the parent Agent Of Control object	Depends on the number of the Agent Of Control objects in the system
4	ID	Enter the value in the field	Sets the unique ID number for the object where <i>Agent of Control</i> is installed	Latin letters and some characters	386	A line representing a sequence of any symbols (letters, digits, service characters excluding characters: space " ", underscore "_", backslash "\" and single quote "'"), not case-sensitive. Number of symbols – from 1 to 9
5	TCP port (UPS)	Enter the value in the field	Sets the port on which to "listen" for UPS messages	Nonnegative integer	8888	from 1 to 60000

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
6	Transmitting...	Click the button	Opens a dialog box with settings for configuring the communication method between <i>Agent of control</i> and <i>Server of control</i>	-	-	-
7	Monitoring...	Click the button	Opens a dialog box for configuring alarm groups	-	-	-
8	Video data...	Click the button	Opens a dialog box for setting video data transferring configurations	-	-	-
9	Cameras	Using the Cameras... button	Displays the list of cameras whose state and archives are monitored by <i>Agent of Control</i> and operating with which shall be available from <i>Monitoring PSIM</i> software interface	-	-	-
10	Cameras..	Click the button	Opens a dialog box for adding cameras for <i>Monitoring PSIM</i>	-	-	-
11	Sensors	Using the Add, Edit and Delete buttons	Displays IDs and types of sensors whose state is monitored by <i>Agent of Control</i> and on whose triggering video data are sent to the Server of Control	-	-	-

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
1 2	Add...	Click the button	Opens a dialog box for adding a sensor. In this dialog box one can also setup video data sending on the sensor triggering	-	-	-
1 3	Edit...	Click the button	Opens a dialog box for editing the sensor. This dialog box is similar to the one for adding a sensor	-	-	-
1 4	Delete	Click the button	Deletes sensor from the list	-	-	-

15.3 Settings panel of the Server Of Control object

Settings panel of the **Server Of Control** object is given on figure.

The screenshot shows the 'Server Of Control' settings panel. It is divided into several sections:

- Top Section:**
 - Field 1: Identifier (value: 1)
 - Field 2: Server Of Control name (value: Server Of Control 1)
 - Field 3: Computer (value: LOCALHOST)
 - Field 4: IIDK interface (value: 150)
 - Field 5: Event Viewer (value: >)
- Logging subsystem:**
 - Field 8: Auxiliary characters
 - Field 9: Alarm events
 - Field 10: System status
 - Field 11: Archive period (h) (value: 48)
 - Field 12: File size (MB) (value: 100)
 - Field 13: Keep archives for (months) (value: 3)
- Advanced:**
 - Field 6: Monitoring ... button
 - Field 7: Snapshots/video ... button
- Transfer:**
 - Field 14: TCP/IP port (Agent) (value: 7777)
 - Field 15: TCP/IP port (Archive) (value: 7755)
 - Field 16: First COM port number (value: Com1)
 - Field 17: Number of COM ports (value: 1)
 - Field 18: COM port speed (value: 9600)
 - Field 19: COM port format (value: 8N1)
- Bottom Section:**
 - Field 20: Transfer info about confirmed alarms to Agent Of Control
 - Field 21: Restart button

At the bottom of the panel are 'Apply' and 'Undo' buttons.

Description of the **Server Of Control** object settings panel elements is given in table.

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
1	Identifier	Automatically	Shows the identification number of the Server Of Control object in the system	Nonnegative integer	-	≥ 0

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
2	Name	Enter the value in the field	Shows the name of the Server Of Control object in the system	Latin letters and service characters	Server Of Control	A line representing a sequence of any symbols (letters, digits, service characters apart from > and < symbols), not case-sensitive. Number of symbols – from 1 to 60
3	Computer	Is selected in the list	Assigns the parent Computer object for the Server Of Control object	Name of the Computer objects registered in the system.	Name of the parent Computer object	Depends on the number of the Computer objects in the system
4	IIDK interface	Enter a value in the field	Sets the ID of the IIDK interface object used by the <i>Server of Control</i>	Nonnegative integer	150	>=0
5	Event Viewer	Click the button	Opens the Event Viewer tool	-	-	-
Advanced group						
6	Monitoring ...	Click the button	Opens the box of setting the list of additional workplaces			
7	Snapshots/ video...	Click the button	Opens a dialog box for configuring reaction to snapshots and videos receiving on sensors alarms at the <i>Agent of Control</i>	-	-	-

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
Logging subsystem group						
8	Auxiliary characters	Is set in a checkbox	Enables logging of auxiliary characters at the transport level into the event log	Boolean	False	True – logging of auxiliary characters is enabled False – logging of auxiliary characters is not performed
9	Alarm events	Is set in a checkbox	Enables logging alarms into the event log	Boolean	True	True – logging of alarms is enabled False – logging of alarms is not performed
10	System status	Is set in a checkbox	Enables logging of events related to system status	Boolean	True	True – logging of events related to system status is enabled False – logging of events related to system status is not performed
11	Archive period (h)	Enter the value in the field	Sets the frequency at which the log file is to be archived	Hours	48	>0
12	File size (MB)	Enter the value in the field	Sets the file size threshold upon which the log file is archived. This setting overrides the value in the Archive period (h) field	Megabytes	100	>0
13	Keep archives for (months)	Enter the value in the field	Sets the length of time for which you want to store archived log files	Months	3	from 1 to 24
Transfer group						

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
14	TCP/IP port (Agent)	Enter the value in the field	Sets the port number for TCP/IP communication with remote objects of Agent Of Control	Nonnegative integer	7777	from 1 to 60000
15	TCP/IP port (Archive)	Enter the value in the field	Sets the port number for TCP/IP communication with remote <i>Search in archive</i> module	Nonnegative integer	7755	from 1 to 60000
16	First COM port number	Is selected in the list	Sets the first COM port number	COM-ports names	Com1	from Com1 to Com 256
17	Number of COM ports	Is selected in the list	Sets number of COM ports used	Nonnegative integer	1	from 1 to 256
18	COM port speed	Is selected in the list	Sets the COM port speed	Baud	9600	110 300 1200 2400 4800 9600 19200 38400 57600

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
19	COM port format	Enter the value in the field	Sets the COM port format	COM port format	8N1	<ul style="list-style-type: none"> • first digit: from 5 to 9 data bits • second letter: N (No parity) – no parity bit, E (Even parity) - even parity bit, O (Odd parity) – odd parity bit • third digit: 1 or 2 stop bits
Outside the groups						
20	Transfer info about confirmed alarms to Agent Of Control	Set the checkbox	Enables sending confirmations of alarm acceptance by the operator on the <i>Server of Control</i> to the <i>Agent of Control</i>	Boolean type	Yes	<p>True – confirmations of alarm acceptance are sent</p> <p>False – confirmations of alarm acceptance are not sent</p>
21	Restart	Click the button	<i>VideoSrv</i> communication module restarting	-	-	-

15.4 Settings panel of the Monitoring interface object

Settings panel of the **Monitoring** interface object is given on figure.


Description of the **Monitoring** object settings panel elements is given in table.

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
1	Identifier	Automatically	Shows the identification number of the Monitoring object in the system	Nonnegative integer	-	≥ 0


#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
2	Name	Enter the value in the field	Shows the identification number of the Monitoring object in the system	Latin letters and service characters	Monitoring	A line representing a sequence of any symbols (letters, digits, service characters apart from > and < symbols), not case-sensitive. Number of symbols – from 1 to 60
3	Display	Is selected in the list	Assigns the parent Display object for the Monitoring object	Names of Display objects registered in the system	Name of the parent Display object	Depends on the number of the Display objects in the system
4	Groups of alarms check boxes	Is set in a check box	Sets alarms that one want to visualize on the Control panel	Boolean	All check boxes except the Extra 1 and Extra 2 are set	If check box is set next to the group of alarms, then alarm from the corresponding group will be displayed on the Control panel
5	Owners panel check box	Is set in a check box	Enables Owners panel displaying	Boolean	True	True – Owners panel is displayed False – Owners panel is hidden

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
	X: field	Enter the value in the field	Set the X coordinate in the horizontal axis for the upper-left corner of the Owners panel interface box	% of the screen width	0	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
	Y: field	Enter the value in the field	Set the Y coordinate in the vertical axis for the upper-left corner of the Owners panel interface box	% of the screen width	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
	W: field	Enter the value in the field	Set the width of the Owners panel interface box	% of the screen width	100	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200


#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
	H: field	Enter the value in the field	Set the height of the Owners panel interface box	% of the screen width	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
	% field	Enter the value in the field	Sets the scaling of objects in the Owners panel	Percent	100	From 100% to 500%. If the scaling parameter exceeds 110%, then the high resolution icons will be displayed on the object, and the Courier New font will be used for the text in the object title, otherwise - MS Sans Serif
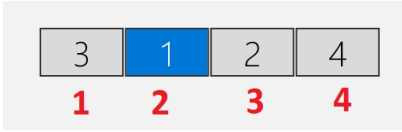
#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
	Monitor drop-down list	Select from the list	<p>Sets the number of the physical monitor which coordinates are specified. Monitors are numbered in physical order from left to right, top to bottom. Thus, number 1 corresponds to the top-left monitor, regardless of which monitor is the primary or first in the OS numbering.</p> <p>In the figure, the monitor numbers in the OS are highlighted in gray, and monitor numbers in <i>Axxon PSIM</i> are highlighted in red:</p>  <p>Attention! It is recommended to use the same resolution for all monitors in the system. Different resolutions are allowed only if each row of logical monitors is aligned to some sort of boundary (for example, to the top)</p>	Natural number series	1	From 1 to 16
6	Control panel check box	Is set in a check box	Enables Control panel displaying	Boolean	True	True – Control panel is displayed False – Control panel is hidden
	X: field	Enter the value in the field	Set the X coordinate in the horizontal axis for the upper-left corner of the Control panel interface box	% of the screen width	0	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
	Y: field	Enter the value in the field	Set the Y coordinate in the vertical axis for the upper-left corner of the Control panel interface box	% of the screen height	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
	W: field	Enter the value in the field	Set the width of the Control panel interface box	% of the screen width	100	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
	H: field	Enter the value in the field	Set the height of the Control panel interface box	% of the screen height	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
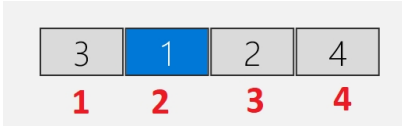
#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
	% field	Enter the value in the field	Sets the scaling of objects in the Control panel	Percent	100	From 100% to 500%. If the scaling parameter exceeds 110%, then the high resolution icons will be displayed on the object, and the Courier New font will be used for the text in the object title, otherwise - MS Sans Serif
	Monitor drop-down list	Select from the list	<p>Sets the number of the physical monitor which coordinates are specified. Monitors are numbered in physical order from left to right, top to bottom. Thus, number 1 corresponds to the top-left monitor, regardless of which monitor is the primary or first in the OS numbering.</p> <p>In the figure, the monitor numbers in the OS are highlighted in gray, and monitor numbers in <i>Axxon PSIM</i> are highlighted in red:</p>  <p>Attention! It is recommended to use the same resolution for all monitors in the system. Different resolutions are allowed only if each row of logical monitors is aligned to some sort of boundary (for example, to the top)</p>	Natural number series	1	From 1 to 16

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
7	Log panel check box	Is set in a check box	Enables Log panel displaying	Boolean	True	True – Log panel is displayed False – Log panel is hidden
	X: field	Enter the value in the field	Set the X coordinate in the horizontal axis for the upper-left corner of the Log panel interface box	% of the screen width	0	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
	Y: field	Enter the value in the field	Set the Y coordinate in the vertical axis for the upper-left corner of the Log panel interface box	% of the screen height	0	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
	W: field	Enter the value in the field	Set the width of the Log panel interface box	% of the screen width	100	from 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
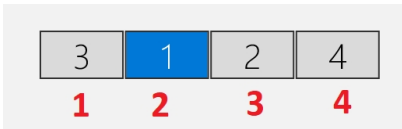
#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
	H: field	Enter the value in the field	Set the height of the Log panel interface box	% of the screen width	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
	Monitor drop-down list	Select from the list	<p>Sets the number of the physical monitor which coordinates are specified. Monitors are numbered in physical order from left to right, top to bottom. Thus, number 1 corresponds to the top-left monitor, regardless of which monitor is the primary or first in the OS numbering.</p> <p>In the figure, the monitor numbers in the OS are highlighted in gray, and monitor numbers in <i>Axxon PSIM</i> are highlighted in red:</p>  <p>Attention! It is recommended to use the same resolution for all monitors in the system. Different resolutions are allowed only if each row of logical monitors is aligned to some sort of boundary (for example, to the top)</p>	Natural number series	1	From 1 to 16


#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
8	Non-empty Comment field check box	Is set in a check box	Is set to require that operators leave comments when accepting an alarm to describe the alarm and/or their actions	Boolean	True	True – Comment field shall not be empty on alarm accepting False – alarm accepting can be done without a comment from Operator
9	Use filter by events check box	Is set in a check box	Is set to enable filtering objects by Alarm and Failure events and Connected and Disconnected states	Boolean	True	True – filter can be applied. False – filter cannot be applied.
10	Warning when watching live video check box	Is set in a check box	Is set if it is necessary to display a warning upon the live video playback attempt that it can create the critical load on the data channel	Boolean	True	True – when live video is attempted to be viewed, the warning is displayed False – when live video is attempted to be viewed, the video is displayed with no warnings
11	Viewing live video through gateway check box	Is set in a check box	Is set if <i>Agents of Control</i> and <i>Additional workplaces</i> are in different subnets and the <i>Monitoring PSIM</i> components are not in a distributed system configuration in <i>Axxon PSIM</i> object tree and Data gateway is in use for transmission of live video to <i>Additional workplaces</i>	Boolean	False	True – live video is transferred to the <i>Additional workplaces</i> through the data gateway False – live video is transferred to the <i>Additional workplaces</i> directly from the <i>Agent of control</i>

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
12	Viewing live video from all cameras (add.) check box	Is set in a check box	Is set if the All cameras of Partition of Control item should be added to the object's Video image playback context menu which enables viewing video from all cameras of the selected <i>Partition of Control</i>	Boolean	False	True – the All cameras of Partition of Control item is added to the object's Video image playback context menu False – there is no All cameras of Partition of Control item in the menu
13	Video stream speed field	Enter the value in the field	Sets the number of frames per second of the video image when viewing live video or video from the archive. <ul style="list-style-type: none"> <i>Note 1. If the archive is recorded with the h264 codec and the video stream speed is set to more than 0 frames per second, then the archive video will be played back only by reference frames</i> <i>Note 2. If the value of the video stream speed is 0, then the live and archive video will be played back without scaling</i> 	Frames per second	25	Depends on the camera features
14	Compression drop-down list	Select from the list	Sets live video compression rate.	Supported compression rates	No	0-5
15	Cameras.. button	Click the button	Opens a window for configuring cameras prohibited from viewing live video for users	-	-	-

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
16	Filter by owners field	Via the Filter... button	Displays selected pairs of users and owners	-	-	-
17	Filter... button	Click the button	Opens a window for configuring the correspondence of owners to users	-	-	-

15.5 Settings panel of the Monitoring reports interface object


Settings panel of the **Monitoring reports** interface object is given on figure.

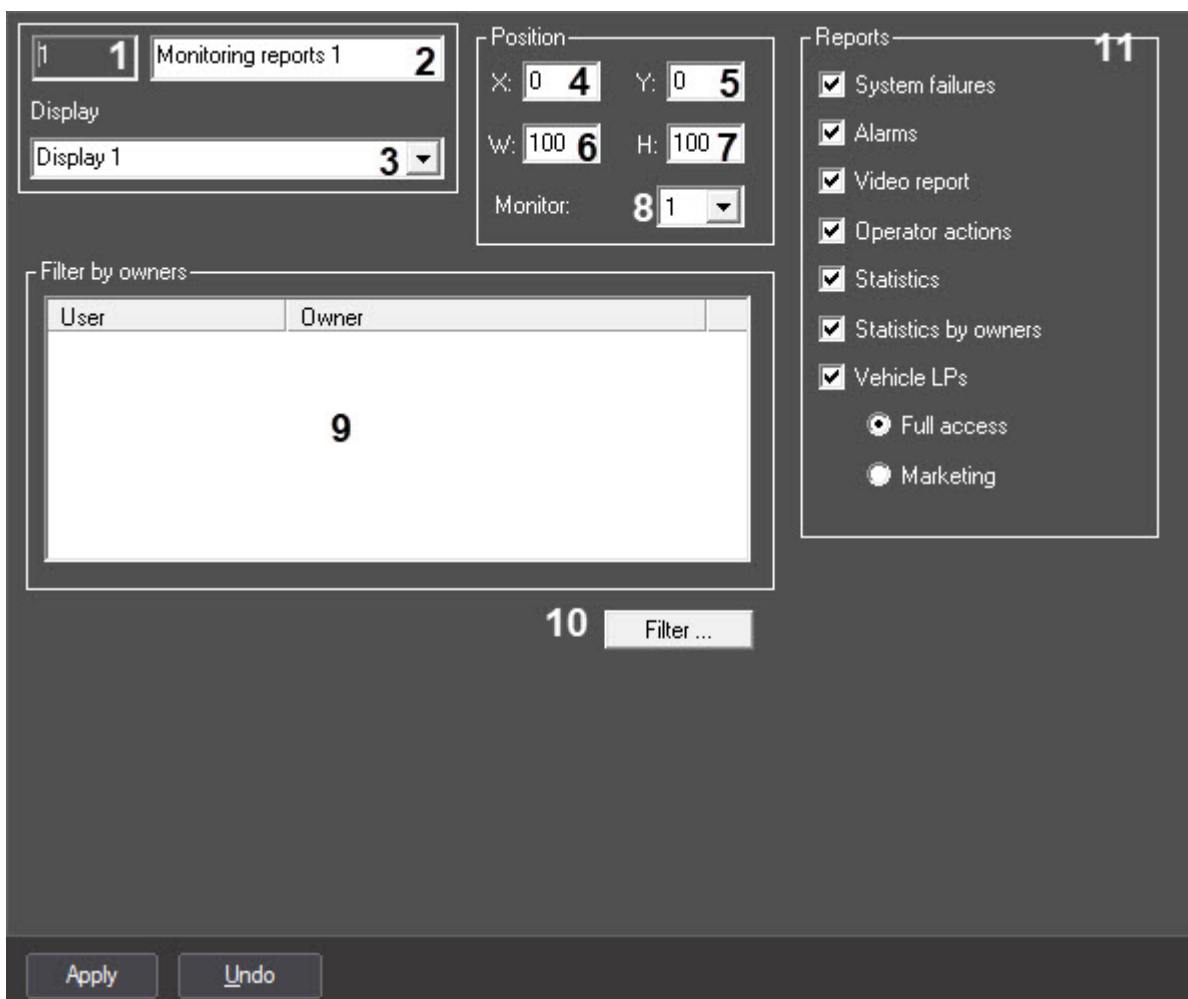

Description of the **Monitoring reports** object settings panel elements is given in table.

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
1	Identifier	Automatically	Shows the identification number of the Monitoring reports object in the system	Nonnegative integer	-	≥ 0
2	Name	Enter the value in the field	Shows the identification number of the Monitoring reports object in the system	Latin letters and service characters	Monitoring reports	A line representing a sequence of any symbols (letters, digits, service characters apart from > and < symbols), not case-sensitive. Number of symbols – from 1 to 60
3	Display	Is selected in the list	Assigns the parent Display object for the Monitoring reports object	Names of Display objects registered in the system	Name of the parent Display object	Depends on the number of the Display objects in the system
4	X:	Enter the value in the field	Set the X coordinate in the horizontal axis for the upper-left corner of the Monitoring reports interface window	% of the screen width	0	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200


#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
5	Y:	Enter the value in the field	Set the Y coordinate in the vertical axis for the upper-left corner of the Monitoring reports interface window	% of the screen height	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
6	W:	Enter the value in the field	Sets width of the Monitoring reports interface window	% of the screen width	100	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
7	H:	Enter the value in the field	Sets height of the Monitoring reports interface window	% of the screen height	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
8	Monitor	Select from the list	<p>Sets the number of the physical monitor which coordinates are specified. Monitors are numbered in physical order from left to right, top to bottom. Thus, number 1 corresponds to the top-left monitor, regardless of which monitor is the primary or first in the OS numbering.</p> <p>In the figure, the monitor numbers in the OS are highlighted in gray, and monitor numbers in <i>Axxon PSIM</i> are highlighted in red:</p>  <p>Attention! It is recommended to use the same resolution for all monitors in the system. Different resolutions are allowed only if each row of logical monitors is aligned to some sort of boundary (for example, to the top)</p>	Nonnegative integer	1	From 1 to 16

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
9	Filter by owners	Via the Filter... button	Displays selected pairs of users and owners	-	-	-
10	Filter...	Click the button	Opens a dialog box to match owners to users	-	-	-
11	Reports	Set the check box	Select reports available in the interface window	Boolean	All check boxes are set, full access to the Vehicle PLs report is set	Yes – the report button is displayed in the Monitoring reports interface window No – the report button is not displayed in the Monitoring reports interface window

15.6 Settings panel of the Search in archive interface object

Settings panel of the **Search in archive** interface object is given on figure.

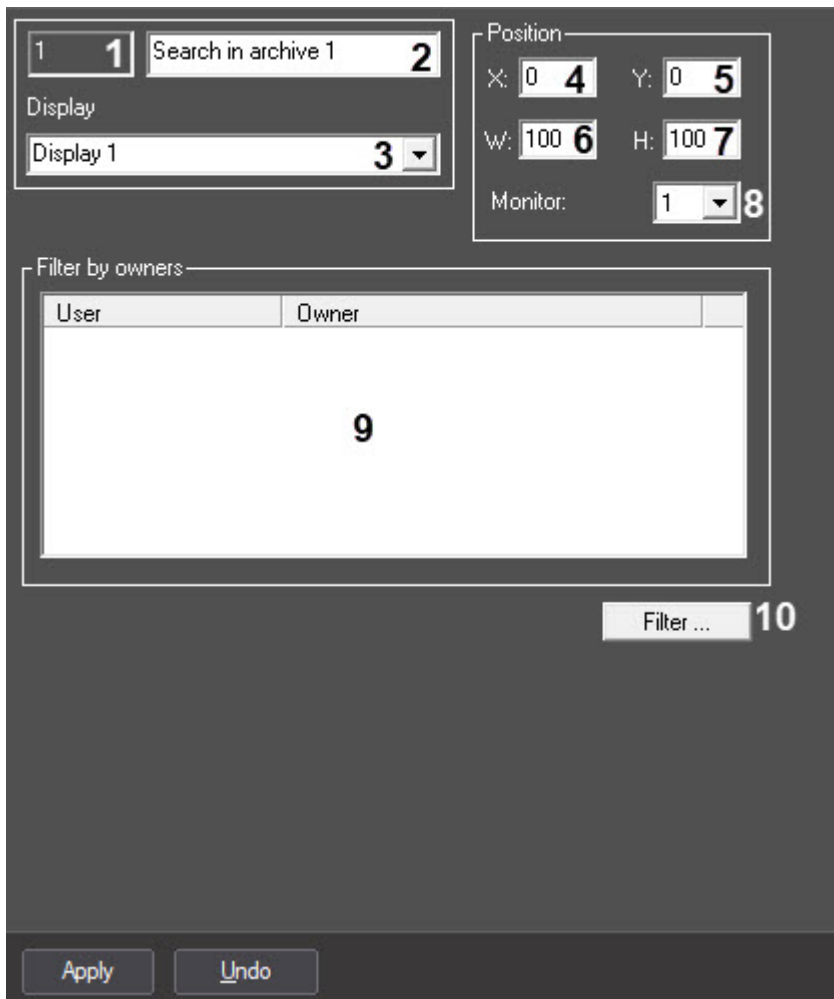


Description of the **Search in archive** object settings panel elements is given in table

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
1	Identifier	Automatically	Shows the identification number of the Search in archive object in the system	Nonnegative integer	-	≥ 0

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
2	Name	Enter the value in the field	Shows the name of the Search in archive object in the system	Latin letters and service characters	Search in archive	A line representing a sequence of any symbols (letters, digits, service characters apart from > and < symbols), not case-sensitive. Number of symbols – from 1 to 60
3	Display	Is selected in the list	Assigns the parent Display object for the Search in archive object	Names of Display objects registered in the system	Name of the parent Display object	Depends on the number of the Display objects in the system
4	X:	Enter the value in the field	Set the X coordinate in the horizontal axis for the upper-left corner of the Search in archive interface box	% of the screen width	0	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
5	Y:	Enter the value in the field	Set the Y coordinate in the vertical axis for the upper-left corner of the Search in archive interface box	% of the screen height	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200


#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
6	W:	Enter the value in the field	Sets width of the Search in archive interface box	% of the screen width	100	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200
7	H:	Enter the value in the field	Sets height of the Search in archive interface box	% of the screen height	50	From 0 to 100. When more than one monitor is connected to the computer it is possible to use coordinates outside this range, but it is not recommended to use coordinates less than -200

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
8	Monitor	Select from the list	<p>Sets the number of the physical monitor which coordinates are specified. Monitors are numbered in physical order from left to right, top to bottom. Thus, number 1 corresponds to the top-left monitor, regardless of which monitor is the primary or first in the OS numbering.</p> <p>In the figure, the monitor numbers in the OS are highlighted in gray, and monitor numbers in <i>Axxon PSIM</i> are highlighted in red:</p>  <p>Attention! It is recommended to use the same resolution for all monitors in the system. Different resolutions are allowed only if each row of logical monitors is aligned to some sort of boundary (for example, to the top)</p>	Nonnegative integer	1	From 1 to 16
9	Filter by owners	Via the Filter... button	Displays selected pairs of users and owners	-	-	-

#	Name	Method for setting the parameter value	Description	Type	Default value	Value range
10	Filter...	Click the button	Opens a window for configuring the correspondence of owners to users	-	-	-

15.7 Settings panel of the Central Server Of Control object

Settings panel of the **Central Server Of Control** object is given on figure.

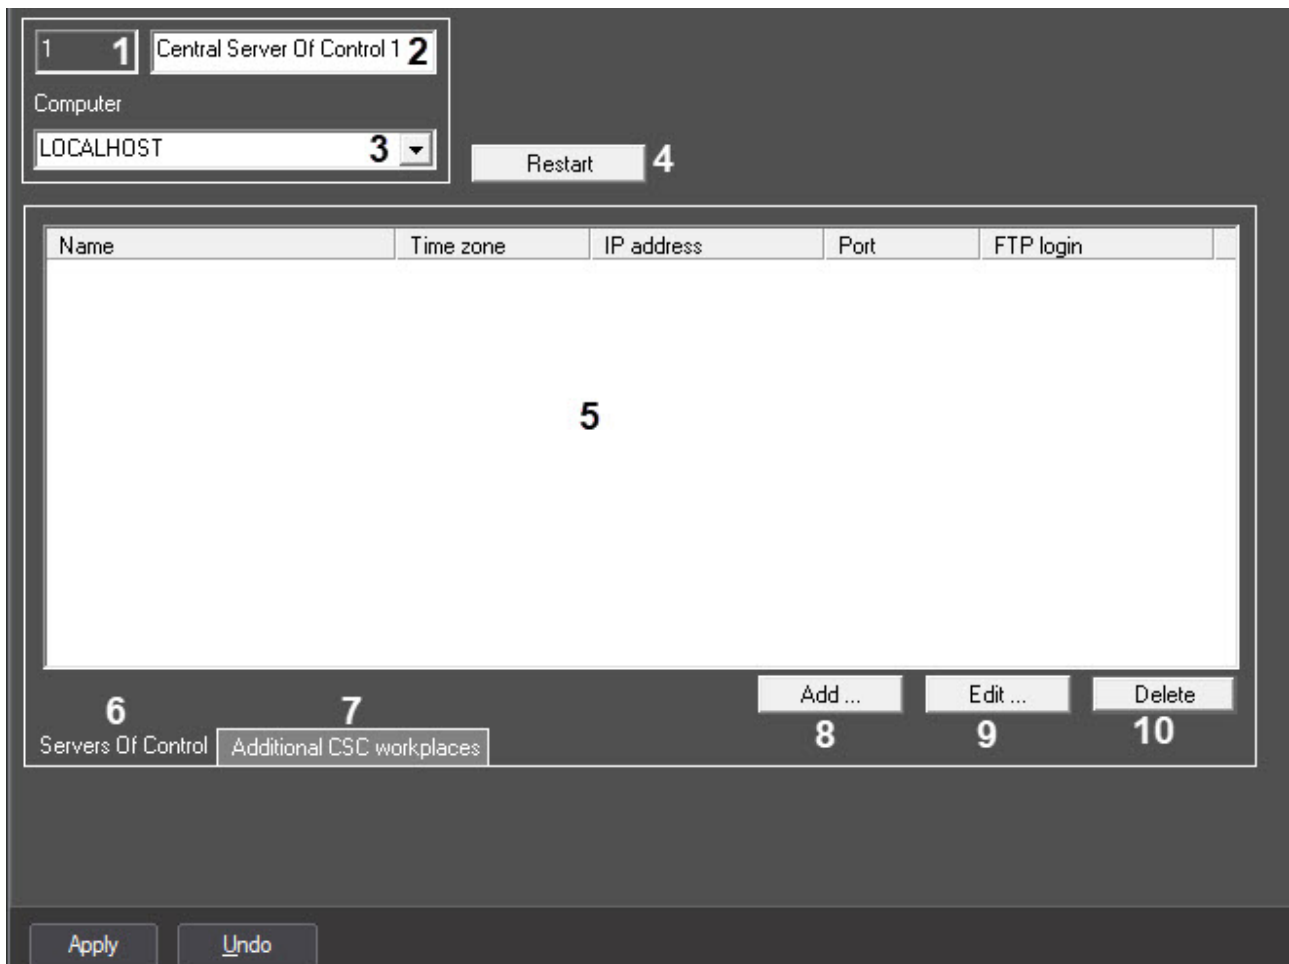

Description of the **Central Server Of Control** object settings panel elements is given in table.

No	Name	Method for setting the parameter value	Description	Type	Default value	Value range
1	Identifier	Automatically	Shows the identification number of the Central Server Of Control object in the system	Nonnegative integer	-	≥ 0
2	Name	Enter the value in the field	Shows the name of the Central Server Of Control object in the system	Latin letters and service characters	Central Server Of Control	A line representing a sequence of any symbols (letters, digits, service characters apart from > and < symbols), not case-sensitive. Number of symbols – from 1 to 60
3	Computer	Select from the list	Assigns the parent Computer object for the Central Server Of Control object	Name of the Computer objects registered in the system	Name of the parent Computer object	Depends on the number of the Computer objects in the system
4	Restart	Click the button	Restart of the CentralNetServer communication module	-	-	-
5	-	-	The table containing the monitored <i>Servers of Control</i> or added <i>Additional workplaces of CSC</i>			
6	Servers Of Control	Click the tab	The tab for configuring and displaying the monitored <i>Servers of Control</i>	-	-	-

№	Name	Method for setting the parameter value	Description	Type	Default value	Value range
7	Additional CSC workplaces	Click the tab	The tab for configuring and displaying the <i>Additional workplaces of CSC</i> which have the permission to be connected to the <i>Central Server of Control</i>	-	-	-
8	Add...	Click the button	The settings window for adding the <i>Server of Control/Additional workplace of CSC</i>	-	-	-
9	Edit...	Click the button	The settings window for editing the parameters of added <i>Servers of Control/Additional workplaces of CSC</i>	-	-	-
10	Delete	Click the button	Deletes the selected <i>Server of Control/Additional workplace of CSC</i>	-	-	-

16 Appendix 2. Sample scripts


16.1 Sample script for processing Server of Control command on Agent of Control

In the *Monitoring PSIM* software package one can configure ad hoc command sending by the Operator of the *Server of Control* to the *Agent of Control*.

Information on how to configure commands on the *Server of Control* can be found in the [Executing ad hoc command on the Agent of Control by the operator of Server of Control](#) section of [Operator's Guide](#).

A script for processing incoming commands is to be created on the *Agent of Control*.

Extra menu items are created on the *Server of Control*: **Arm Camera 1** and **Disarm Camera 1**. They send a command with parameter 1 or 2 correspondently.

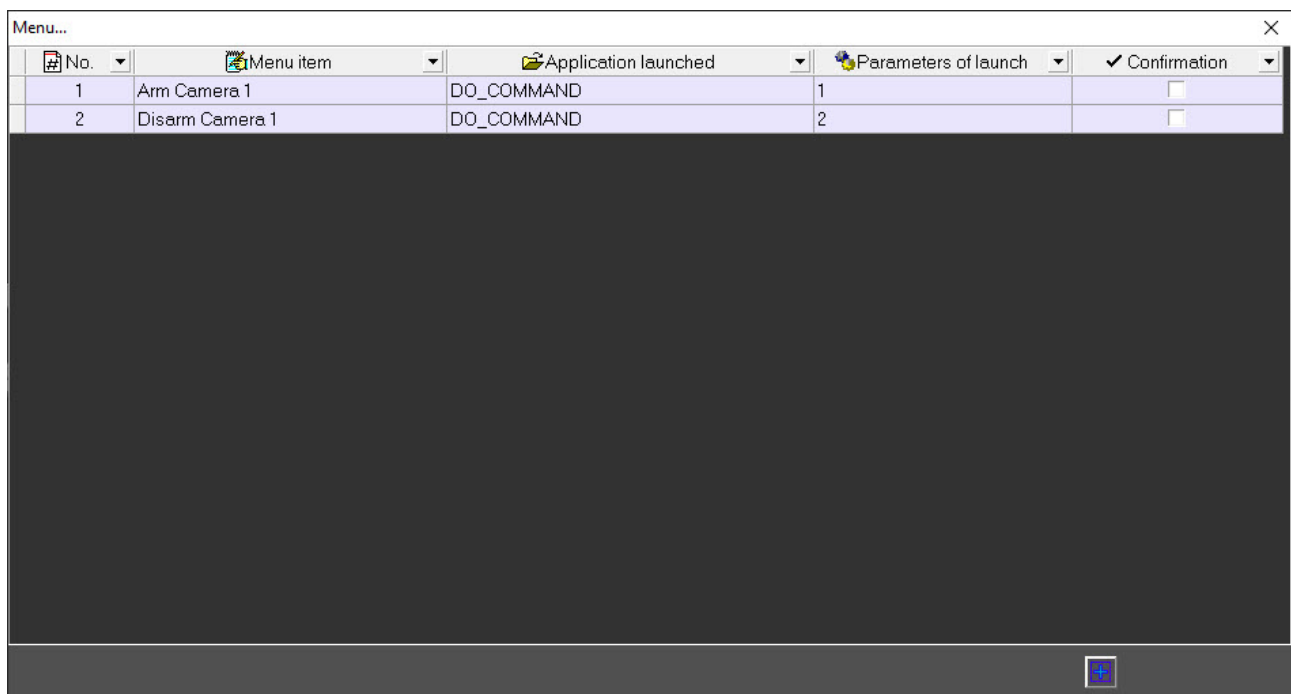

The sample of program in *Axxon PSIM* embedded language for processing the incoming command is shown below:

```
OnEvent("VIDEOSRV_C_DVC", "1", "DO_COMMAND")
{
  if (strequal(param0, "1"))
  {
    DoReact("CAM", "1", "ARM");
  }
  if (strequal(param0, "2"))
  {
    DoReact("CAM", "1", "DISARM");
  }
}
```

16.2 Sample script for setting custom filter in the Log panel

Custom filter on the **Log panel** can be changed with a script or macro. For more details on the filter and its configuration in the user interface, see [Custom filter in the Log panel](#).

Use APPLY_FILTER reaction of the VIDEOSRV_M object to create or change the custom filter in the **Log panel**:

```
DoReact("VIDEOSRV_M", "", "APPLY_FILTER", "computer<>, query<>");
```

Parameters:

computer<> – NetBIOS name of the computer to execute the command on.

query<> – filter condition.

The query<>parameter syntax:

query<TotalExpressions;BoolOperatorKind;Expression[;Expression]>

- **TotalExpressions** — number of expressions in the condition

Example:

TotalExpressions = 1 for condition (Cameras equal 2)

TotalExpressions = 3 for condition (Cameras equal 2) and ((Disks equal 1) or (Disks equal 2))

- **BoolOperatorKind** — boolean operator for main expression. Possible values:

– and

– or

Example:

BoolOperatorKind = and for condition (Cameras equal 2)

BoolOperatorKind = and for condition (Cameras equal 2) and ((Disks equal 1) or (Disks equal 2))

BoolOperatorKind = or for condition (Cameras equal 1) or (Cameras equal 2)

- **Expression** — one or several expressions

Format: Field;Expressions;LocalBoolOperator;OperatorKind;Value

- *Field* — name of the field in the DB table.

Possible values:

– ID

– Name

– Region

– Province

– City

– CamCnt

– ArcMax

– HddCnt

– IpAddress

– FirstRecord

– TemperHdd

– AvailMemory

– WorkingTime

– VerSoft

- *Expressions* — number of expressions in a subcondition.

Example:

Expressions = 1 for condition (Cameras equal 2) and ((Disks equal 1) or (Disks equal 2))

Expressions = 2 for condition (Cameras equal 2) and ((Disks equal 1) or (Disks equal 2))

- *LocalBoolOperator* — boolean operator for subconditions. Possible values:

– and

– or

Example:

LocalBoolOperator = and for condition (Cameras equal 2)

LocalBoolOperator = or for condition (Cameras equal 2) and ((Disks equal 1) or (Disks equal 2))

- *OperatorKind* – operator type.
Possible values:
 - Equal
 - NotEqual
 - Less
 - LessOrEqual
 - Greater
 - GreaterOrEqual
 - Like
 - NotLike
- *Value* – value to compare with.

Examples:

(Cameras equal 2) ▼

query<1;and;CamCnt;1;and;Equal;2>

With main expressions:

(Cameras less 5) AND (Cameras greater 3) ▼

query<2;and;CamCnt;1;and;Less;5;CamCnt;1;and;Greater;3>

With subquery:

((Cameras less 5) AND (Cameras greater 3)) ▼

query<2;and;CamCnt;2;and;Less;5;CamCnt;2;and;Greater;3>

((Cameras greater 1) AND (Cameras less 5) AND (Disks greater 0)) ▼

query<3;and;CamCnt;2;and;Greater;1;CamCnt;2;and;Less;5;HddCnt;1;and;Greater;0>

(Name ending with 47) ▼

query<1;and;Name;1;and;Like;%47>

16.3 Sample script for stopping camera recording

If you want for a JPEG still frame to be attached to an alarm message or video fragment when a sensor is activated (**Sensor** object), remember that this is possible only after the current archive file has been written to disk. To reduce the waiting time (the **Delay (sec.)** parameter, see the section [Configuring sensors](#)) and be assured of camera recording, you can create a **Program** object on the **Programming** tab of *Axxon PSIM* software package.

These programs are written for a camera with an ID of 1 and for a **Sensor** object whose ID is also equal to 1. Thanks to these programs, the value of the **Delay** parameter can be set equal to 7 seconds.

⚠ Attention!

To get several video fragments, you can specify several repeated commands "REC" and "REC_STOP" in the script. If "rollback" is used, and the prerecording time in the settings of the **Camera** object is greater than or equal to the time between subsequent "REC_STOP" and "REC" commands, then this video fragment will be combined with the next video fragment.

Option 1. The camera is disarmed:

```
OnEvent("GRAY","1","ALARM")
{
[
  if( !CheckState("CAM","1","DETACHED") )
  {
    DoReact("CAM","1","REC","rollback<1>");
    Wait(5);
    DoReact("CAM","1","REC_STOP","priority<2>");
  }
]
}

```

```
OnEvent("GRAY","1","ALARM")
{
[
  Wait(2);
  DoReact("GRAY","1","CONFIRM");
  Wait(2);
  DoReact("GRAY","1","ARM");
]
}
```

Option 2. Camera is armed:

```
OnEvent("GRAY","1","ALARM")
{
[
  if( !CheckState("CAM","1","DETACHED") )
  {
    DoReact("CAM","1","DISARM");
    Sleep(50);
    DoReact("CAM","1","REC","rollback<1>");
    Wait(5);
    DoReact("CAM","1","REC_STOP","priority<2>");
    Sleep(2050); // Prerecording time in the Camera settings = 2 sec.
    DoReact("CAM","1","ARM");
  }
]
}

```

```
OnEvent("GRAY","1","ALARM")
{
```

```
[
  Wait(2);
  DoReact("GRAY","1","CONFIRM");
  Wait(2);
  DoReact("GRAY","1","ARM");
]
}
```

Option 3. Continuous recording:

```
OnEvent("GRAY","1","ALARM")
{
  [
    if( !CheckState("CAM","1","DETACHED") )
    {
      Wait(5); // Specifies the time after which the recording should be stopped in
order to get the required video fragment or number of frames
      DoReact("CAM","1","REC_STOP","priority<2>");
      Sleep(2050); // Prerecording time in the Camera settings = 2 sec.
      DoReact("CAM","1","REC","rollback<1>"); // Start recording with 2 sec
rollback (during prerecording). Thus, data in the archive is not lost.
    }
  ]
}

```

```
OnEvent("GRAY","1","ALARM")
{
  [
    Wait(2);
    DoReact("GRAY","1","CONFIRM");
    Wait(2);
    DoReact("GRAY","1","ARM");
  ]
}
```

16.4 Sample scripts for processing alarm confirmations

The **Partition Of Control** object (VIDEOSRV_C_DVC) sends the «Confirm: Event of monitoring» (CONF_MON) message to *Axxon PSIM* core when an alarm is confirmed.

When the confirmation type is **Simple**, then param0<> has the same value as the ID of event that is confirmed (see [Configuration for associating events with certain alarm groups](#) section). When **param1<>** is **0**, it means that a Simple confirmation is used.

Below you will find a sample program that can be written on the *Agent Of Control* in order to process a received simple confirmation. As a result a camera is armed.

```
OnEvent("VIDEOSRV_C_DVC","1","CONF_MON")
{
  if (strequal(param0,"1"))
  {
```

```
DoReact("CAM","1","ARM");
}
}
```

When the confirmation type is **Complex**, then param0<> has the value of the ID of event that is confirmed (see [Configuration for associating events with certain alarm groups](#) section). If param1<> is **1**, it means that the operator has clicked the **OK** button in the confirm box. If the operator clicked the **Cancel** button, then param1<> would be **2**.

Below you will find a sample program that can be written on the *Agent of Control* in order to process a received complex confirmation. As a result a camera is armed only when the operator clicks the **OK** button in the confirm box.

```
OnEvent("VIDEOSRV_C_DVC","1","CONF_MON")
{
  if (strequal(param0,"1")&&strequal(param1,"1"))
  {
    DoReact("CAM","1","ARM");
  }
}
```

16.5 Sample script to export filtered data from the Log panel to .xls

Before executing this command, apply filter in the **Log panel**. It can be done from the user interface (see [Custom filter in the Log panel](#)) or by a script (see [Sample script for setting custom filter in the Log panel](#)).

Export filtered **Log panel** data to the test.xls file on disk C:

```
DoReact("VIDEOSRV_M","", "EXPORT_EXCEL", "computer<NamePC>,file<c:\test.xls>");
```

16.6 Sample script to show and hide Search license plates window

Show **Search license plates** window with 70% screen width and 50% screen height in the upper left of the display:

```
DoReact("VIDEOSRV_M","", "SHOW_AUTO", "computer<NamePC>,x<0>,y<0>,w<70>,h<50>");
```

Hide **Search license plates** window:

```
DoReact("VIDEOSRV_M","", "HIDE_AUTO", "computer<NamePC>");
```

Parameters:

computer<> – name of the computer to execute command on.

x<> – X-axis coordinate of upper left corner the window.

y<> – Y-axis coordinate of upper left corner the window.

w<> – window width as a percentage of the screen width.

h<> – window height as a percentage of the screen height.

16.7 Sample scripts for the special mode of Monitoring PSIM operation with ACFA PSIM

16.7.1 Sample script for configuring the interaction between the Monitoring PSIM and the Apollo integration module

This script records the users from the *Server of Control* side into the *Apollo* integration module, which is installed on the *Agent of Control* side.

Attention!

The configuration guide for the *Apollo* integration module is available in the documentation for *ACFA PSIM*. This script can be modified for any other integration module that supports user entry into the controller.

Note

For details, see [Configuring the special mode of Monitoring PSIM operation with ACFA PSIM](#).

```
function SetPersons(srcDepartment, destTable, destTableSize, msg)
{
    var users = CreateMsg();
    users.StringToMsg(GetObjectIds("PERSON"));
    var userCount = users.GetParam("id.count");
    var i;
    var index;
    for(i = 0, index = 1; (index <= destTableSize) && (i < userCount); ++i)
    {
        var user = users.GetParam("id." + i);
        if(GetObjectParentId("PERSON", user, "DEPARTMENT") == srcDepartment)
        {
            msg.SetParam("USERS.user_id." + Itv_var("counter"), user);
            msg.SetParam("USERS.number." + Itv_var("counter"), index);
            msg.SetParam("USERS.key_type." + Itv_var("counter"), destTable);
            index++;
            Lock();
            Itv_var("counter")++;
            Unlock();
        }
    }
}

if(Event.SourceType == "VIDEOSRV_C" && Event.Action == "SPR_DATA_UPDATED")
{
    var APOLLO_TYPE = "APOLLO_DEVICE";
    var APOLLO_ID = "1.1";
    var WRITE_CONFIG_REACT = "WRITE_CONFIG";
    Itv_var("counter") = 0;
    var msg = CreateMsg();
    msg.SourceType = "CORE";
    msg.SourceId = "";
```

```

msg.Action = "UPDATE_OBJECT";
msg.SetParam("objtype", APOLLO_TYPE);
msg.SetParam("objid", APOLLO_ID);
var type = GetObjectParam(APOLLO_TYPE, APOLLO_ID, "type");
if(type == "A6")
{
    SetPersons("1", "USER", 79, msg);
}
else
{
    SetPersons("1", "USER", 255, msg);
}
SetPersons("2", "POLICE", 15, msg);
SetPersons("3", "ELECTRIC", 15, msg);

msg.SetParam("USERS.user_id.count", Itv_var("counter"));
msg.SetParam("USERS.number.count", Itv_var("counter"));
msg.SetParam("USERS.key_type.count", Itv_var("counter"));
NotifyEvent(msg);
NotifyEventStr(APOLLO_TYPE, APOLLO_ID, WRITE_CONFIG_REACT, "");
}

```

16.7.2 Sample scripts for determining the current state of the zones of the Apollo object on the Agent of Control side

This script determines the current state of the zones on the *Agent of Control* side with the configured *Apollo* integration module. Also, when the **GET_OBJECT_STATE** event is received, this script generates the **OBJECT_STATE_INFO** event. The zones are configured and assigned to the corresponding loops when configuring the *Apollo* integration module.

Attention!

The configuration guide for the *Apollo* integration module is available only in the documentation for *ACFA PSIM*. This script can be modified for any other integration module that supports user entry into the controller.

Note

For details, see [Configuring the special mode of Monitoring PSIM operation with ACFA PSIM](#).

```

function GetStateByCounts(armedCount, disarmedCount)
{
    /* If there are both armed and disarmed zones, then we consider that arming is
    partially completed */
    if(armedCount > 0 && disarmedCount > 0)
    {
        return "PART_ARMED";
    }
    /* If there are only armed zones, then we consider that the controller is armed
    */
}

```

```

else if(armedCount > 0)
{
    return "ARMED";
}
/* We consider that the controller is disarmed */
return "DISARMED"
}
function ZoneIsUsed(params, id)
{
    var count = params.GetParam("TABLE.zone.count");
    var number = GetObjectParam("APOLLO_ZONE", id, "number");
    var i;
    for(i=0; i < count; ++i)
    {
        if(params.GetParam("TABLE.zone." + i) == number)
        {
            return "true";
        }
    }
    return "false";
}
function GetControllerState(id, zones)
{
    /* Get the controller configuration*/
    var params = CreateMsg();
    params.StringToMsg(GetObjectParams("APOLLO_DEVICE", id));
    /* Get the number of zones used by the controller */
    var count = params.GetParam("TABLE.zone.count");
    /* If the controller uses the zones */
    if(count > 0)
    {
        /* The number of armed and disarmed zones */
        var armedCount = 0;
        var disarmedCount = 0;
        var zoneCount = zones.GetParam("id.count");
        var j;
        for(j = 0; j < zoneCount; ++j)
        {
            /* Determine if the zone belongs to the current controller
            and determine whether this zone is used by the current controller */
            var zone = zones.GetParam("id."+j);
            if(GetObjectParentId("APOLLO_ZONE", zone, "APOLLO_DEVICE") == id &&
ZoneIsUsed(params, zone) == "true")
            {
                /* Check the state of the zone */
                var state = GetObjectState("APOLLO_ZONE", zone);
                switch(state)
                {
                    case "ARMED":
                    case "ALARM_ARMED":
                    case "TROUBLE_ARMED":
                        armedCount++;
                        break;

```

```

        case "DISARMED":
        case "TROUBLE_DISARMED":
            disarmedCount++;
            break;
        }
    }
}

/* Check the state of the object */
return GetStateByCounts(armedCount, disarmedCount, msg);
}
function GetSkdStateMsg(type, id, action)
{
    var devices = CreateMsg();
    devices.StringToMsg(GetObjectIds("APOLLO_DEVICE"));
    var count = devices.GetParam("id.count");
    var zones = CreateMsg();
    zones.StringToMsg(GetObjectIds("APOLLO_ZONE"));
    /* The number of armed and disarmed zones */
    var armedCount = 0;
    var disarmedCount = 0;
    var i;
    for(i = 0; i < count; ++i)
    {
        var device = devices.GetParam("id."+i);
        var state = GetControllerState(device, zones);
        switch(state)
        {
            case "PART_ARMED":
                disarmedCount++;
            case "ARMED":
                armedCount++;
                break;
            case "DISARMED":
                disarmedCount++;
                break;
        }
    }
    var msg = CreateMsg();
    msg.SourceType = type;
    msg.SourceId = id;
    msg.Action = action;

    msg.SetParam("state", GetStateByCounts(armedCount, disarmedCount));
    msg.SetParam("card", "");
    return msg;
}
if(Event.SourceType == "VIDEOSRV_C" && Event.Action == "GET_OBJECT_STATE")
{
    NotifyEvent(GetSkdStateMsg(Event.SourceType, Event.SourceId, "OBJECT_STATE_INFO")
);
}

```

```

else if(Event.SourceType == "APOLLO_DEVICE" &&
(Event.Action == "A06_CLOSE" ||
Event.Action == "A16_CLOSE" ||
Event.Action == "A06_OPEN" ||
Event.Action == "A16_OPEN" ||
Event.Action == "A06_POLICE" ||
Event.Action == "A16_POLICE" ||
Event.Action == "A06_ELECTRIC" ||
Event.Action == "A16_ELECTRIC" ||
Event.Action == "A06_ENTRY" ||
Event.Action == "A16_ENTRY"))
{
    var card = Event.GetParam("key_code");
    var msg = GetSkdStateMsg("VIDEOSRV_C", "1", "OBJECT_STATE_INFO");
    msg.SetParam("card", card);
    NotifyEvent(msg);
}

```

16.8 Sample scripts for determining the current state of the relay on the Agent of Control side

This script determines the current state of the relay on the *Agent of Control* side. Also, when the **GET_OBJECT_STATE** event is received, this script generates the **OBJECT_STATE_INFO** event (for details, see [Configuring alarms for monitoring object's state on the Agent of Control side](#)). Using the **card** parameter from the *Agent of Control*, it is possible to transfer any additional information to the *Server of Control*. This information will be displayed in the **Event log** (see [Event log](#)).

```

function GetReleStateMsg(type, id, action, card)
{
    var state = GetObjectState("GRELE","1");
    var msg = CreateMsg();
    msg.SourceType = type;
    msg.SourceId = id;
    msg.Action = action;
    msg.SetParam("state", (state=="OFF")?"DISARMED":"ARMED");
    msg.SetParam("card", card);
    return msg;
}

if(Event.SourceType=="VIDEOSRV_C" && Event.SourceId=="1" && Event.Action=="GET_OBJECT_STATE")
{
    NotifyEvent(GetReleStateMsg(Event.SourceType, Event.SourceId, "OBJECT_STATE_INFO", ""));
}
else if(Event.SourceType=="GRELE" && (Event.Action=="ON" || Event.Action=="OFF"))
{
    NotifyEvent(GetReleStateMsg("VIDEOSRV_C", "1", "OBJECT_STATE_INFO", ""));
}

```

16.9 Sample script for creating a hardware failures report

A **Hardware failures report** (see [System failures](#)) can be automatically generated using a script that uses the REPORT_FAILURES reaction of the VIDEOSRV_R object:

```
DoReact("VIDEOSRV_R", "", "REPORT_FAILURES", "computer<>,file<>,export<>,object<>,region<>,district<>,city<>,type<>,fromTime<>,toTime<>,sorting<>,comment<>");
```

Parameters description is given in the table below:

Parameter	Description
computer<>	Specifies the NetBIOS name of the computer on which the report is to be created. Required parameter.
file<>	The full path to the file where the report will be saved. Required parameter.
export<>	Format of the export file. 0 - Excel, 1 - HTML, 2 - RTF, 3 - CSV. Optional parameter. If this parameter is absent, the file is exported in Excel format.
object<>	The object on which the report is created. This parameter specifies the "Object code", which is displayed on the Log Panel of the Monitoring PSIM interface object (see Information about an object). Optional parameter. If this parameter is absent, a report is created for all objects.
region<>	Filter by the Region. It is necessary to specify the indexing numbers of the options to be used separated by commas in the Region drop-down list. For example: (region<1,3>) (see System failures). Optional parameter. If this parameter is absent, a report is created for all regions.
district<>	Filter by the District. It is necessary to specify the indexing numbers of the options to be used separated by commas in the District drop-down list. For example: (district<2,3,5>) (see System failures). Optional parameter. If this parameter is absent, a report is created for all districts.

Parameter	Description
city<>	Filter by the City. It is necessary to specify the indexing numbers of the options to be used separated by commas in the City drop-down list. For example: (city<1>) (see System failures). Optional parameter. If this parameter is absent, a report is created for all cities.
type<>	Filter by the Failure type. It is necessary to specify the indexing numbers of the options to be used separated by commas in the Failure type drop-down list. For example: (type<1,3,5>) (see System failures). Optional parameter. If this parameter is absent, a report is created for all failure types.
fromTime<>	Date and time of the report beginning in the DD-MM-YY HH:MM:SS format. Required parameter.
toTime<>	Date and time of the report ending in the DD-MM-YY HH:MM:SS format. Required parameter.
sorting<>	Sorting mode. 0 - by event, 1 - by time. Optional parameter. If this parameter is absent, sorting by event is used.
comment<>	Show comment. 0 - do not show, 1 - show. Optional parameter. If this parameter is absent, comments are not shown.

Sample script that will automatically create a **Hardware failures report** every day at 20:00 and save it to the C:\report.html file:

```
OnTime(W,D,X,Y,"20","00","00")
{
  DoReact("VIDEOSRV_R","", "REPORT_FAILURES", "computer<Monitoring>,file<c:\report.html>,export<1>,fromTime<" + date + " 00:00:00>,toTime<" + date + " " + time + ">");
}
```

16.10 Sample script for creating an alarms report

An **Alarms report** (see [Alarms](#)) can be automatically generated using a script that uses the REPORT_ALARMMS reaction of the VIDEOSRV_R object:

```
DoReact("VIDEOSRV_R", "", "REPORT_ALARMS", "computer<>,file<>,export<>,object<>,region<>,district<>,city<>,type<>,fromTime<>,toTime<>,sorting<>,comment<>,filter<>");
```

Parameters description is given in the table below:

Parameter	Description
computer<>	Specifies the NetBIOS name of the computer on which the report is to be created. Required parameter.
file<>	The full path to the file where the report will be saved. Required parameter.
export<>	Format of the export file. 0 - Excel, 1 - HTML, 2 - RTF, 3 - CSV. Optional parameter. If this parameter is absent, the file is exported in Excel format.
object<>	The object on which the report is created. This parameter specifies the "Object code", which is displayed on the Log Panel of the Monitoring interface object (see Information about an object). Optional parameter. If this parameter is absent, a report is created for all objects.
region<>	Filter by the Region. It is necessary to specify the indexing numbers of the options to be used separated by commas in the Region drop-down list. For example: (region<1,3>) (see Alarms). Optional parameter. If this parameter is absent, a report is created for all regions.
district<>	Filter by the District. It is necessary to specify the indexing numbers of the options to be used separated by commas in the District drop-down list. For example: (district<2,3,5>) (see Alarms). Optional parameter. If this parameter is absent, a report is created for all districts.
city<>	Filter by the City. It is necessary to specify the indexing numbers of the options to be used separated by commas in the City drop-down list. For example: (city<1>) (see Alarms). Optional parameter. If this parameter is absent, a report is created for all cities.

Parameter	Description
type<>	Filter by the Alarm type. It is necessary to specify the indexing numbers of the options to be used separated by commas in the Alarm drop-down list. For example: (type<1,3,5>) (see Alarms). Optional parameter. If this parameter is absent, a report is created for all alarm types.
fromTime<>	Date and time of the report beginning in the DD-MM-YY HH:MM:SS format. Required parameter.
toTime<>	Date and time of the report ending in the DD-MM-YY HH:MM:SS format. Required parameter.
sorting<>	Sorting mode. 0 - by event, 1 - by time. Optional parameter. If this parameter is absent, sorting by event is used.
comment<>	Show comment. 0 - do not show, 1 - show. Optional parameter. If this parameter is absent, comments are not shown.
filter<>	Text filter by messages of monitored alarms (see Configuring alarm groups). Optional parameter.

Sample script that will automatically create an **Alarms report** every day at 20:00 and save it to the C:\report.html file:

```
OnTime(W,D,X,Y,"20","00","00")
{
DoReact("VIDEOSRV_R","", "REPORT_ALARMS", "computer<Monitoring>,file<c:\report.html>,export<1>,fromTime<" + date + " 00:00:00>,toTime<" + date + " " + time + ">");
}
```